



Sentara Williamsburg Community Hospital
301 Monticello Avenue
Williamsburg, Virginia 23185

April 14, 2005

Michelle Beardsley, Health Physicist - Medical Branch
Division of Nuclear Materials Safety
United States Nuclear Regulatory Commission
Region I - Division of Nuclear Materials Safety
475 Allendale Road
King of Prussia, Pennsylvania 19406

RE: Amend License 45-16209-02 03014703

Sentara Williamsburg Community Hospital would like to amend our NRC materials' license number 45-16209-02 to add an additional area of use. We would like to be able to inject of ^{99m}Tc (Sulfur Colloid) for sentinel node imaging of the breast at our Women's Imaging Pavilion located in our Outpatient Care Center (OCC) on 6601 Mooretown Road, Williamsburg, VA. The procedures used for the injection and biopsy will be identical to those used in the hospital. The patient will be imaged and the biopsy will be performed in the OR of the OCC. We will purchase a dose calibrator, well counter and a survey meter so that we can perform all of the required assessments under our license. We are altering one of our mammographic imaging rooms to allow for receipt, administration and decay in storage. Please see attached diagram.

If you have any questions regarding this amendment please contact me at (757) 259-6074.

Sincerely,

Maureen S. Green

Maureen S. Green, RTRM, CRA
Radiology Manager

RECEIVED
REGION 1
APR 15 2:35

136880
NMSS/RGNI MATERIALS-002

V-112
72.6

V-125
72.1

V-126
75.5

V-114
71.6

V-105
71.7

Control Booth

Mammography Unit

Counter Cabinets

LEAD STORAGE


DOSE CAL

WELL

V-102
72.2


V-101

V-124
74.2

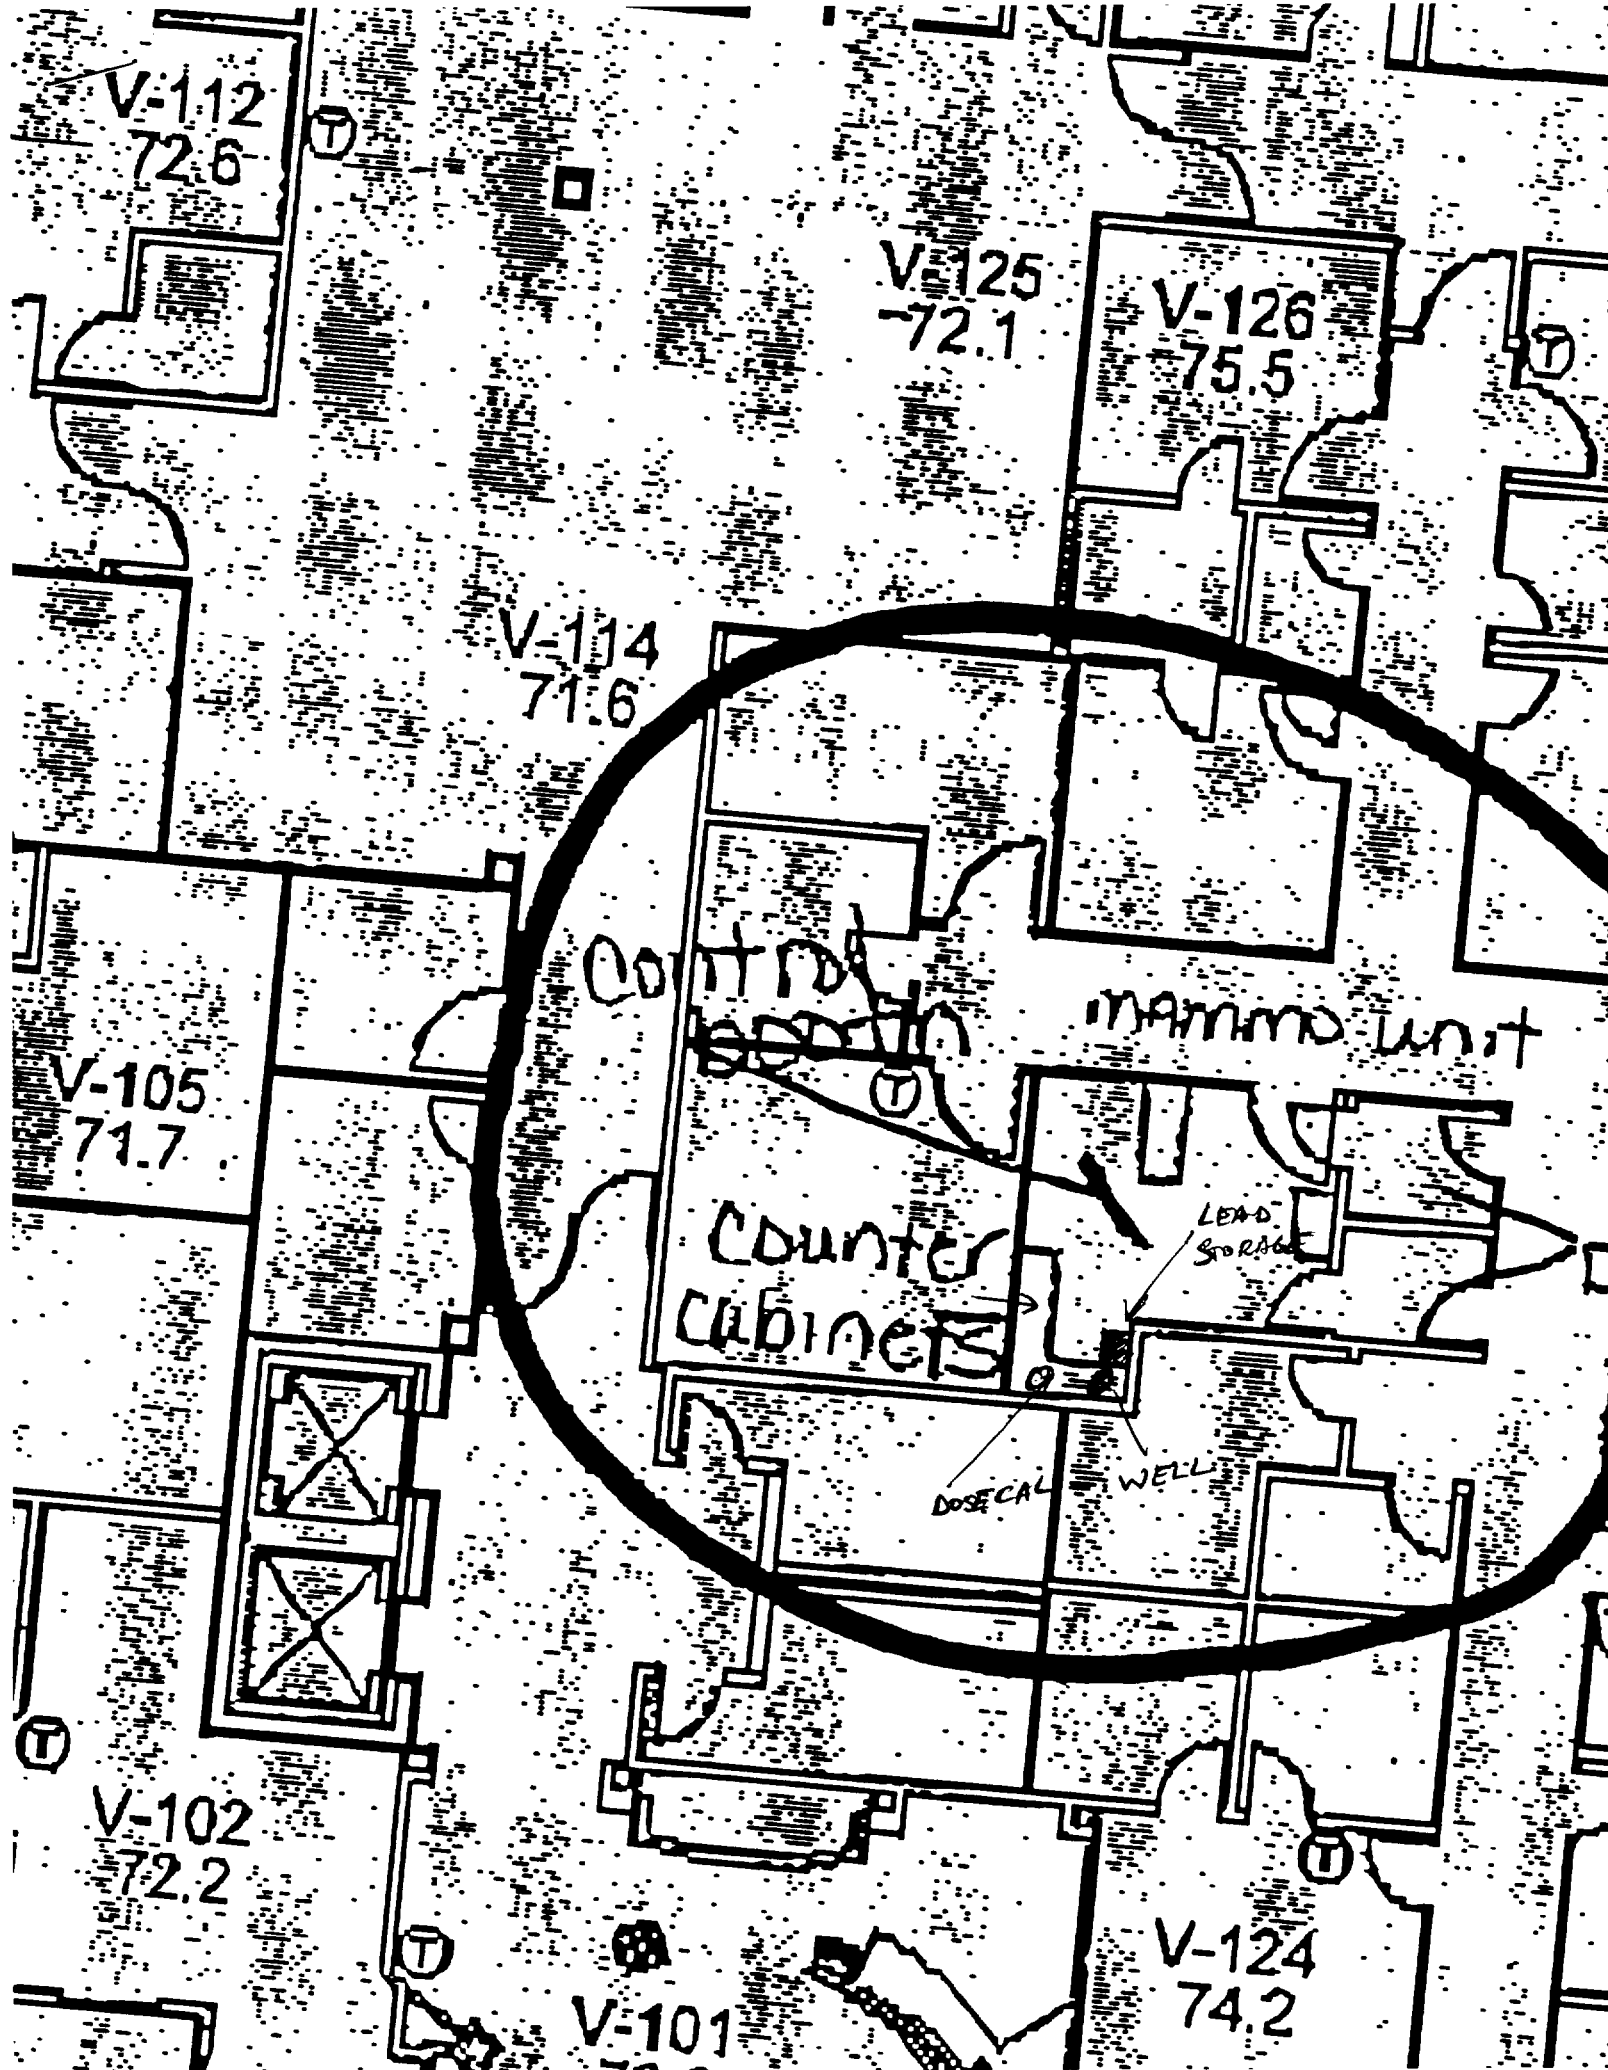

001/001

04/13/2005 WED 16:30 FAX 757 3454001 Womens Imaging Pavilion →→→ XRAY

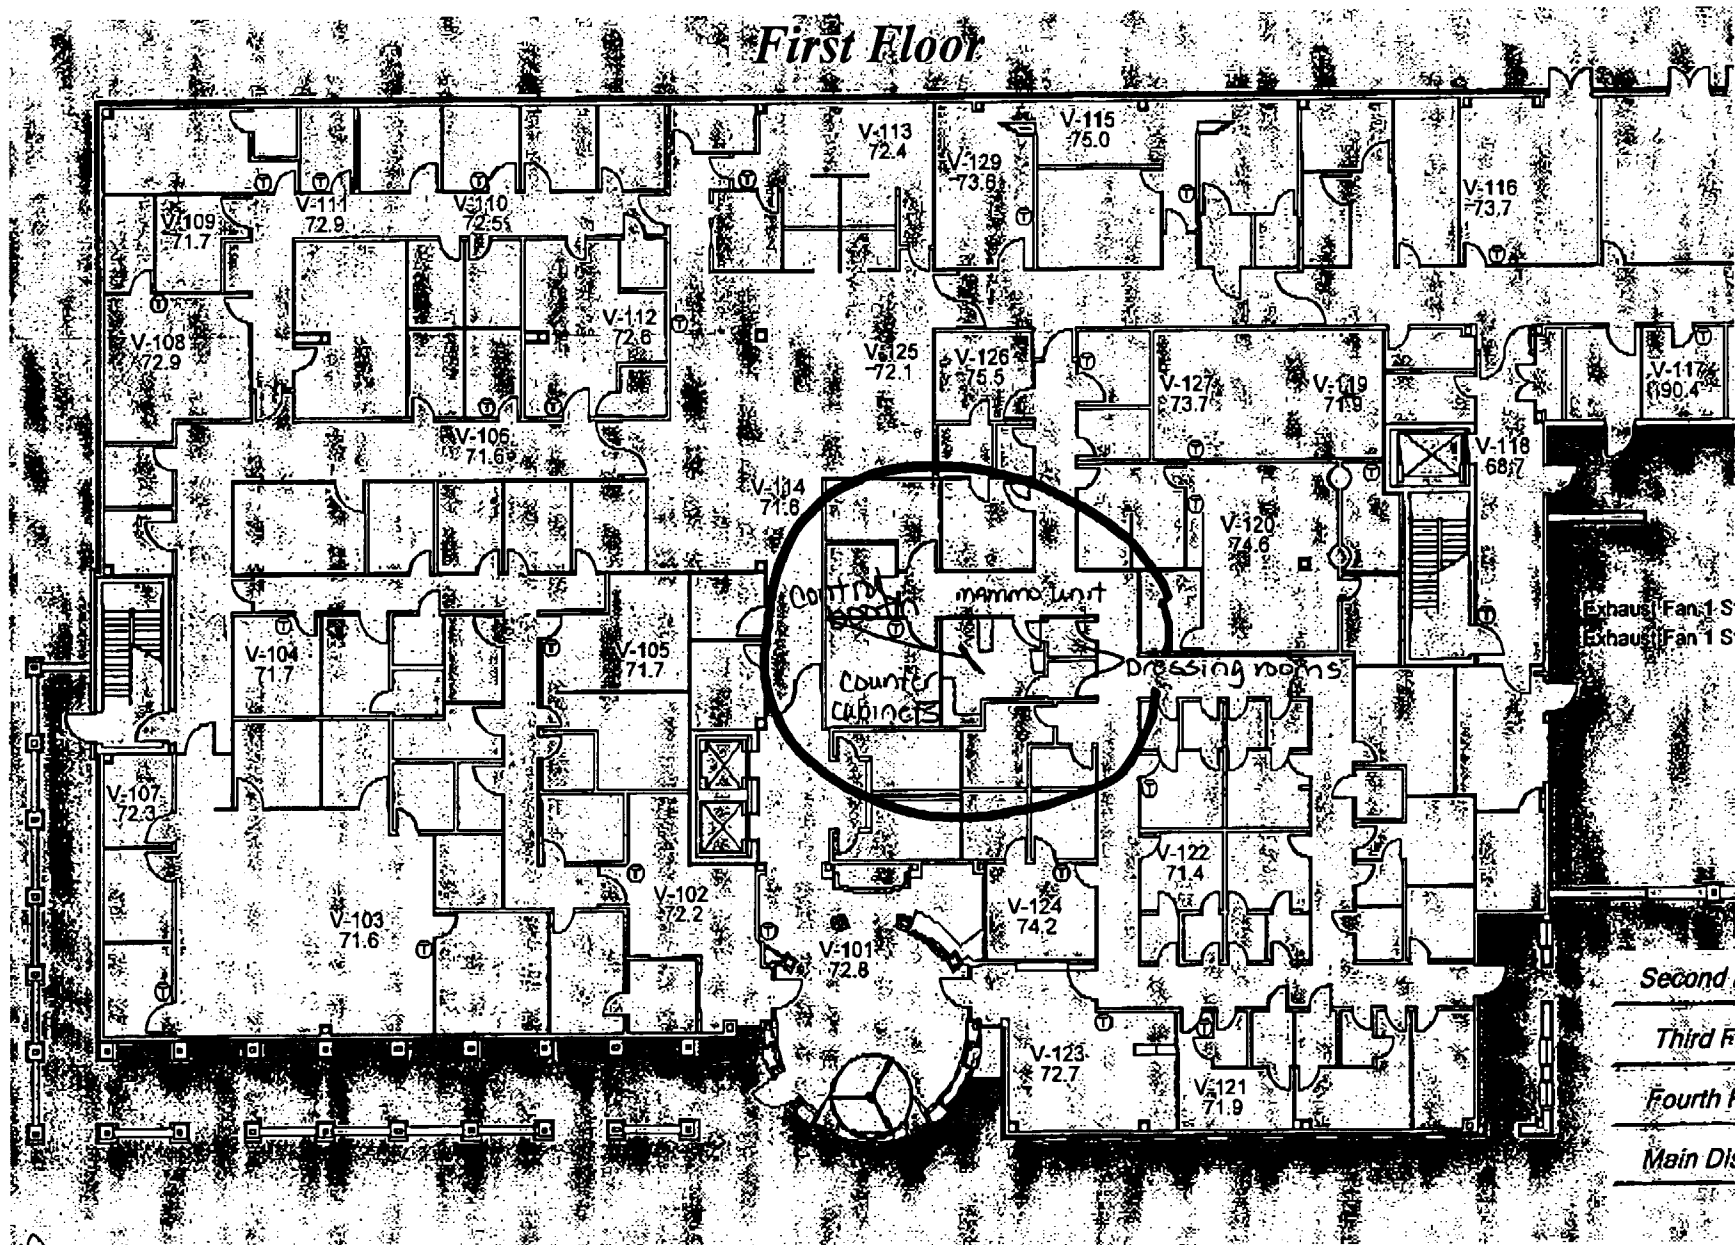

Alec

Donna

Womens Imaging Pavilion
OCC/SWELL

This is to acknowledge the receipt of your letter/application dated

4/14/2005, and to inform you that the initial processing which includes an administrative review has been performed.

☒ Amendment 45-16209-02
There were no administrative omissions. Your application was assigned to a technical reviewer. Please note that the technical review may identify additional omissions or require additional information.

☐ Please provide to this office within 30 days of your receipt of this card

A copy of your action has been forwarded to our License Fee & Accounts Receivable Branch, who will contact you separately if there is a fee issue involved.

Your action has been assigned **Mail Control Number** 136880.
When calling to inquire about this action, please refer to this control number.
You may call us on (610) 337-5398, or 337-5260.

BETWEEN: : (FOR LFMS USE)
: INFORMATION FROM LTS
: -----
:
License Fee Management Branch, ARM : Program Code: 02120
and : Status Code: 0
Regional Licensing Sections : Fee Category: 7C
: Exp. Date: 20141231
: Fee Comments: CODE 23
: Decom Fin Assur Req'd: N
:

LICENSE FEE TRANSMITTAL

A. REGION I

1. APPLICATION ATTACHED

Applicant/Licensee: SENTARA WILLIAMSBURG COMMUNITY HOSP
Received Date: 20050415
Docket No: 3014703
Control No.: 136880
License No.: 45-16209-02
Action Type: Amendment

2. FEE ATTACHED

Amount: /
Check No.: /

3. COMMENTS

Signed [Signature]
Date 4/22/05

B. LICENSE FEE MANAGEMENT BRANCH (Check when milestone 03 is entered /__/)

1. Fee Category and Amount: _____

2. Correct Fee Paid. Application may be processed for:

Amendment _____
Renewal _____
License _____

3. OTHER _____

Signed _____
Date _____