

# REID HOSPITAL AND HEALTH CARE SERVICES.

## FAX TRANSMISSION COVER PAGE

**FAX PHONE NUMBER: (765) 983-3260**

DATE: 10-21-05

TIME: \_\_\_\_\_

TO: Bill Reichhold

LOCATION: Nuclear Regulatory Commission, Region III

FAX NUMBER: 630-829-9782

DEPARTMENT: \_\_\_\_\_

NUMBER OF PAGES: 4  
(INCLUDING COVER PAGE)

SPECIAL INSTRUCTIONS: \_\_\_\_\_

### CONFIDENTIALITY NOTICE:

THE DOCUMENTS ACCOMPANYING THIS TELECOPY TRANSMISSION MAY CONTAIN CONFIDENTIAL INFORMATION. THE INFORMATION IS INTENDED ONLY FOR THE USE OF THE INDIVIDUAL(S) OR ENTITY NAMED ABOVE. IF YOU ARE NOT THE INTENDED RECIPIANT, YOU ARE NOTIFIED THAT ANY DISCLOSURE, COPYING, DISTRIBUTION OR THE TAKING OF ANY ACTION IN RELIANCE ON THE CONTENTS OF THIS TELECOPIED INFORMATION IS NOT PERMISSIBLE. IF YOU HAVE RECEIVED THIS TELECOPY IN ERROR, PLEASE IMMEDIATELY NOTIFY US AT (765) 983-3164 TO ARRANGE FOR THE RETURN OF THE ORIGINAL DOCUMENTS. THANK YOU!

REID HOSPITAL AND HEALTH CARE SERVICES  
1401 CHESTER BLVD.  
RICHMOND IN 47374  
(765) 983-3164



October 21, 2005

Bill Reichardt  
Materials Licensing Section  
U.S. Nuclear Regulatory Commission, Region III  
2443 Warrenville Road, Suite 210  
Lisle, Illinois 60532-4352

Mail Control Number 314735

NRC License Number 13-03284-02 for Reid Hospital & Health Care Services

Mr. Reichardt

Please allow this letter to serve as a response to your request for additional information concerning our recent license amendment submission. Our responses follow the same order as your information requests.

1. Our Radiation Safety Officer, Mr. Charles Narayanan, M.S., D.A.B.R., has an office at our hospital location, where the majority of his duties and responsibilities are located. The staff at the proposed location of use will be informed that Mr. Narayanan is the Radiation Safety Officer and how to reach him should there be a matter that requires the attention of the Radiation Safety Officer. In addition, the Radiation Safety Officer, or his delegate at Reid, or his delegate which may include an outside physics consultant, will visit the proposed location of use at least on a quarterly basis. Incidents or emergencies involving radioactive materials at either location of use will take the precedence of the Radiation Safety Officer and will be responded to as soon as is necessary.
2. Physically, the proposed location of use is approximately five minutes from the hospital, by public roads. The staff at the proposed location of use will be informed of who the Radiation Safety Officer is and the contact information; and they will be encouraged to contact him should there be any incident, emergency, or question concerning radioactive materials.
3. The current Reid management will provide oversight for NRC licensed activities at both Reid facilities.



4. We do not currently anticipate the transportation of radioactive materials between the two locations of use. Should such transportation become necessary, all provisions of 10 CFR 71 will be adhered to, and the NRC will be informed prior to such occurrence.
5. We do not currently anticipate sharing radiation safety equipment between the two locations of use. We do reserve the right to share equipment should it become necessary, such as in responding to an emergency or incident involving radioactive materials. We confirm that each location of use will have a dose calibrator, a sodium iodide well detector, a GM survey meter, appropriate shielding materials, and any other equipment necessary to meet all regulatory requirements.
6. The use of radioactive materials at the proposed location of use will be limited to those regulated by 10 CFR 35.100 and 35.200. Please see the enclosed facility diagram.

If additional information is required, please contact:

Gene DiTullio, Director of Radiology Services, Phone: 765-983-3166

Charles Mangum, Radiation Safety Officer, Phone: 765-983-3168

For fax communication, my fax number is 765-983-3260

Sincerely,

*Eugene DiTullio*  
Eugene DiTullio  
Director of Radiology Services

For fax communication, my fax number is 765-983-3260

Sincerely,

*Eugene DiTullio*

Eugene DiTullio  
Director of Radiology Services

1401 Chester Boulevard  
Richmond, Indiana 47374  
www.reidhoep.com  
(765) 983-3099

REID HOSPITAL & HEALTH CARE SERVICES  
OUTPATIENT RADIOLOGY  
OFFICE  
1501 CHESTER BOULEVARD  
RICHMOND, VA 23215-0267

# FACILITIES & EQUIPMENT DIAGRAM


## KEY:

1. SURVEY EQUIPMENT
2. WALL COUNTER/EXCEPT PRINTER
3. SIGN
4. LOCKABLE DOOR
5. CASE RECEIPT AREA
6. L-SHIELD
7. KEY/DOOR PREP AREA
8. ISOTOPE STORAGE
9. UNDER COUNTER WASTE STORAGE
10. DOSE CALIBRATOR
11. WASTE STORAGE
12. DIGITAL CAMERA/CAMERA

13. WALL IN HOT LAB
14. STORAGE CLOSET
15. COMPUTER/CONSOLE
16. DESK
17. FILE CABINET
18. CHAIR CART

## ADJACENT ROOMS

- A. READING ROOM
- B. ECHO STRESS LAB
- C. NUCLEAR TREADMILL RM.
- D. PATIENT EXAM ROOM 1
- E. PATIENT EXAM ROOM 2
- F. HALLWAY
- G. NUCLEAR CAMERA RM.
- H. HOT LAB
- I. LOCKABLE DOORS

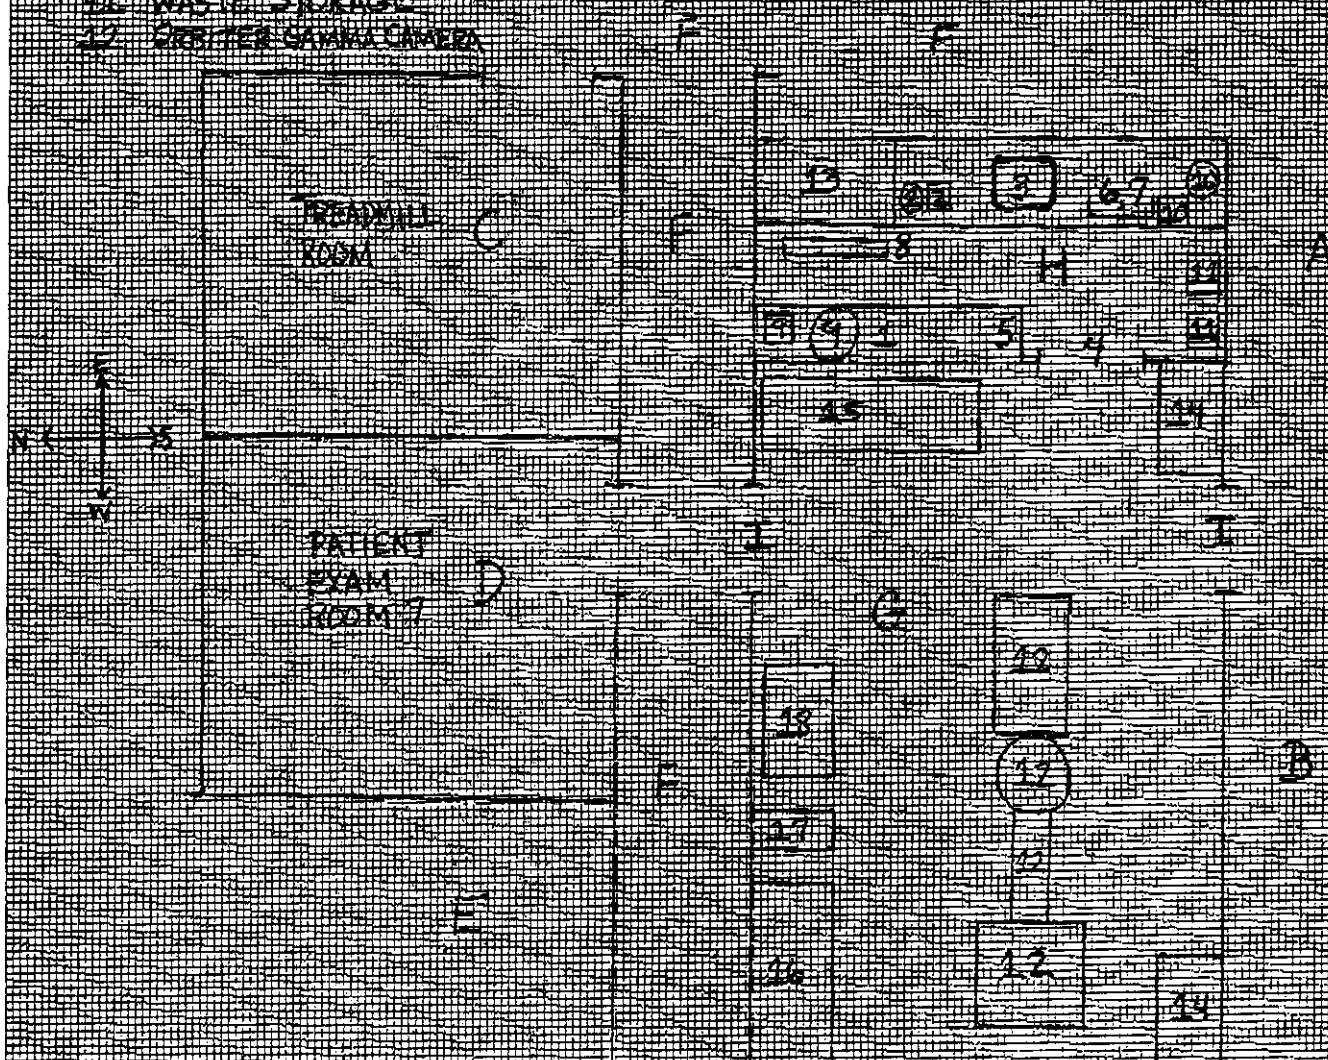

SCALE:

1" = 1 foot

All the area except F (hallway) are restricted areas.  
No occupancy above the stairs.

File storage below the floor.

10/20/2005

# REID HOSPITAL AND HEALTH CARE SERVICES.

## FAX TRANSMISSION COVER PAGE

**FAX PHONE NUMBER: (765) 983-3260**

**DATE:** 10-21-05

**TIME:** \_\_\_\_\_

**TO:** Bill Reichhold

**LOCATION:** Nuclear Regulatory Commission, Region III

**FAX NUMBER:** 630-829-9782

**DEPARTMENT:** \_\_\_\_\_

**NUMBER OF PAGES:** 4  
(INCLUDING COVER PAGE)

**SPECIAL INSTRUCTIONS:**

**CONFIDENTIALITY NOTICE:**

THE DOCUMENTS ACCOMPANYING THIS TELECOPY TRANSMISSION MAY CONTAIN CONFIDENTIAL INFORMATION. THE INFORMATION IS INTENDED ONLY FOR THE USE OF THE INDIVIDUAL(S) OR ENTITY NAMED ABOVE. IF YOU ARE NOT THE EXTENDED RECIPIANT, YOU ARE NOTIFIED THAT ANY DISCLOSURE, COPYING, DISTRIBUTION OR THE TAKING OF ANY ACTION IN RELIANCE ON THE CONTENTS OF THIS TELECOPIED INFORMATION IS NOT PERMISSIBLE. IF YOU HAVE RECEIVED THIS TELECOPY IN ERROR, PLEASE IMMEDIATELY NOTIFY US AT (765) 983-3164 TO ARRANGE FOR THE RETURN OF THE ORIGINAL DOCUMENTS. THANK YOU!

REID HOSPITAL AND HEALTH CARE SERVICES  
1401 CHESTER BLVD.  
RICHMOND IN 47374  
(765) 983-3164



October 21, 2005

Bill Reichhold  
Materials Licensing Section  
U.S. Nuclear Regulatory Commission, Region III  
2443 Warmville Road, Suite 210  
Lisle, Illinois 60532-4352

Mail Control Number 314735

NRC License Number 13-03284-02 for Reid Hospital & Health Care Services

Mr. Reichhold:

Please allow this letter to serve as a response to your request for additional information concerning our recent license amendment submission. Our responses follow the same order as your information requests.

1. Our Radiation Safety Officer, Mr. Charles Narayanan, M.S., D.A.B.R., has an office at our hospital location, where the majority of his duties and responsibilities are located. The staff at the proposed location of use will be informed that Mr. Narayanan is the Radiation Safety Officer and how to reach him should there be a matter that requires the attention of the Radiation Safety Officer. In addition, the Radiation Safety Officer, or his delegate at Reid, or his delegate which may include an outside physics consultant, will visit the proposed location of use at least on a quarterly basis. Incidents or emergencies involving radioactive materials at either location of use will take the precedence of the Radiation Safety Officer and will be responded to as soon as is necessary.
2. Physically, the proposed location of use is approximately five minutes from the hospital, by public roads. The staff at the proposed location of use will be informed of who the Radiation Safety Officer is and the contact information, and they will be encouraged to contact him should there be any incident, emergency, or question concerning radioactive materials.
3. The current Reid management will provide oversight for NRC licensed activities at both Reid facilities.





4. We do not currently anticipate the transportation of radioactive materials between the two locations of use. Should such transportation become necessary, all provisions of 10 CFR 71 will be adhered to, and the NRC will be informed prior to such occurrence.
5. We do not currently anticipate sharing radiation safety equipment between the two locations of use. We do reserve the right to share equipment should it become necessary, such as in responding to an emergency or incident involving radioactive materials. We confirm that each location of use will have a dose calibrator, a sodium iodide well detector, a GM survey meter, appropriate shielding materials, and any other equipment necessary to meet all regulatory requirements.
6. The use of radioactive materials at the proposed location of use will be limited to those regulated by 10 CFR 35.100 and 35.200. Please see the enclosed facility diagram.

If additional information is required, please contact:

Gene DiTullio, Director of Radiology Services, Phone: 765-983-3166

Charles Marayanan, Radiation Safety Officer, Phone: 765-983-3168

For fax communication, my fax number is 765-983-3260

Sincerely,

A handwritten signature in cursive script that reads "Eugene DiTullio".

Eugene DiTullio  
Director of Radiology Services



REID HOSPITAL & HEALTH CARE SERVICES  
OUTPATIENT RADIOLOGY  
OFFICE  
1501 CHESTER BOULEVARD  
RICHMOND, IN 47375-1267

FACILITIES & EQUIPMENT DIAGRAM


KEY:

1. Survey Equipment
2. WELL COUNTER/RECORD PRINTER
3. Sink
4. LOCKABLE DOOR
5. CRT RECEIPT AREA
6. L-SHIELD
7. KIT/DOSE PREP AREA
8. ISOTOPE STORAGE
9. UNDER COUNTER WASTE STORAGE
10. DOSE CALIBRATOR
11. WASTE STORAGE
12. COUNTER GAMMA CAMERA

13. WALL IN HOT LAB
14. STORAGE CLOSET
15. COMPUTER/CONSOLE
16. Desk
17. FILE CABINET
18. CRASH CART

ADJACENT ROOMS:

- A. READING ROOM
- B. ECHO STRESS LAB
- C. NUCLEAR TREADMILL RM.
- D. PATIENT EXAM ROOM 3
- E. PATIENT EXAM ROOM 3
- F. HALLWAY
- G. NUCLEAR CAMERA RM.
- H. HOT LAB
- I. LOCKABLE DOORS

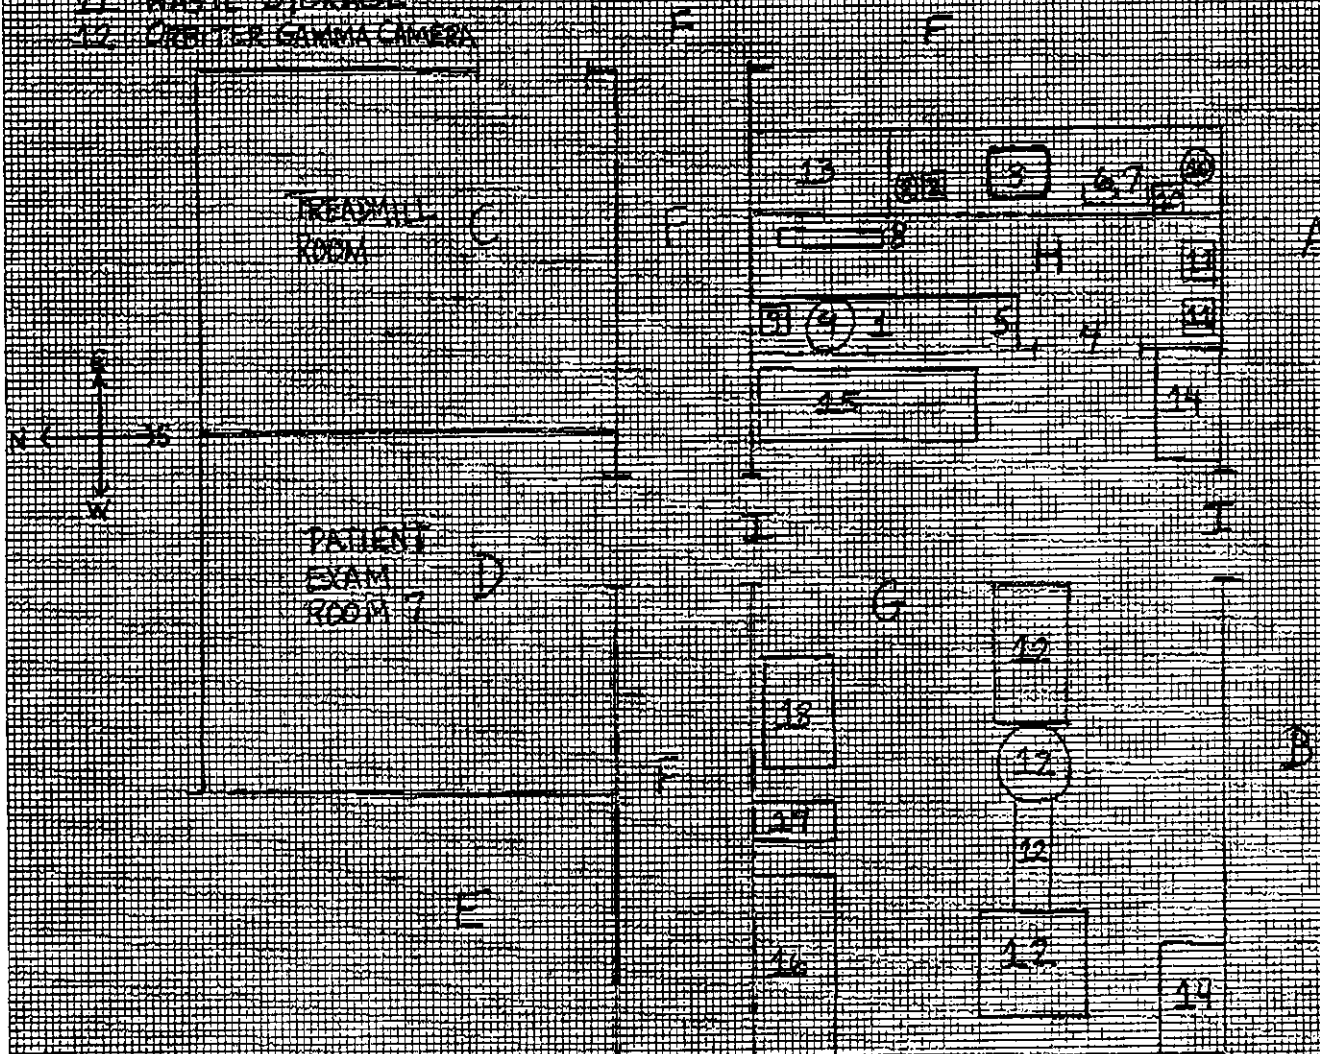

SCALE:  
1" = 1 foot

All the area except F (hallway) are restricted areas  
No occupancy above the stairs

File Storage below the floor

10/20/2005

# REID HOSPITAL AND HEALTH CARE SERVICES.

## FAX TRANSMISSION COVER PAGE

**FAX PHONE NUMBER: (765) 983-3260**

**DATE:** 10-25-05

**TIME:** \_\_\_\_\_

**TO:** Bill Reichhold

**LOCATION:** Nuclear Regulatory Commission Region III

**FAX NUMBER:** 630-829-9782

**DEPARTMENT:** 2

**NUMBER OF PAGES:** \_\_\_\_\_  
(INCLUDING COVER PAGE)

**SPECIAL INSTRUCTIONS:** \_\_\_\_\_

**CONFIDENTIALITY NOTICE:**

THE DOCUMENTS ACCOMPANYING THIS TELECOPY TRANSMISSION MAY CONTAIN CONFIDENTIAL INFORMATION. THE INFORMATION IS INTENDED ONLY FOR THE USE OF THE INDIVIDUAL(S) OR ENTITY NAMED ABOVE. IF YOU ARE NOT THE INTENDED RECIPIANT, YOU ARE NOTIFIED THAT ANY DISCLOSURE, COPYING, DISTRIBUTION OR THE TAKING OF ANY ACTION IN RELIANCE ON THE CONTENTS OF THIS TELECOPIED INFORMATION IS NOT PERMISSIBLE. IF YOU HAVE RECEIVED THIS TELECOPY IN ERROR, PLEASE IMMEDIATELY NOTIFY US AT (765) 983-3164 TO ARRANGE FOR THE RETURN OF THE ORIGINAL DOCUMENTS. THANK YOU!

REID HOSPITAL AND HEALTH CARE SERVICES  
1401 CHESTER BLVD.  
RICHMOND IN 47374  
(765) 983-3164



October 25th, 2006

Bill Reichhold  
Materials Licensing Section  
U.S. Nuclear Regulatory Commission, Region III  
2443 Warranville Road, Suite 210  
Lisle, Illinois 60532-4352

Mail Control Number 314735

NRC License Number 13-03284-02 for Reid Hospital & Health Care Services

Mr. Reichhold:

The additional clarification that you requested:

1. Any delegate or outside consultant will report any findings or issues to the Radiation Safety Officer. The findings or issues will be reported to the Radiation Safety Officer verbally or in writing, as the situation requires. Any issues or findings that need to be brought to the attention of the Radiation Safety Committee will be done so.
2. The staff at the proposed location of use will contact the Radiation Safety Officer by phone. The staff will be provided with both the hospital phone number and the home phone number of the Radiation Safety Officer.
3. The doors to the Nuclear Camera Room are labeled "Nuclear". There is no room number.

The door to the Hot Lab is labeled "Caution Radioactive Materials" and has the radiation symbol. There is no room number.

The treadmill room does not have a room number.

If any additional information is required, please contact:

Eugene DiTullio, Director of Radiology Services, 765-983-3166  
Charles Narayanan, Radiation Safety Officer, 765-983-3188

Sincerely,

*Eugene DiTullio*  
Eugene DiTullio

Director of Radiology Services