


Room 1201 Scoping Survey

Contents

Page

- 2 Floor Plan
- 3 Drawing of a typical 6-foot fume hood
- 4 Wipe test data for Hood 76
- 5 Wipe test data for Hood 78





Floor Plan Room 1201

19 Pendleton Drive
Hebron, CT 06248
(860) 228-0487

Typical 6-Foot Transite Fume Hood

6 Foot fume hood



The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

Attachment A

Report No. Report 3

Customer: Chemtura

Customer Samp No. N/A

Location: 1201 Hood 76

RSA Lab Sample No. N/A

Project: Lab Decommissioning

Date Collected: 3/9/2011

Samp. Description: Survey wipes

Date Counted: 3/9/2011

Matrix: Wipes

C-14 LLD dpm= 39.41

[illegible]

4

Page 1 of 1

Customer: Chemtura

Location: 1201 Hood 78

Project: Lab Decommissioning

Samp. Description: Survey Wipes

Matrix: Wipes

[illegible]


5

Room 1202 Scoping Survey

Contents


Page

- 2 Floor Plan
- 3 Drawing of a typical 6-foot fume hood
- 4 Drawing of a typical 8-foot fume hood
- 5 Wipe test data for Hood A
- 6 Wipe test data for Hood B
- 7 Wipe test data for Hood C



RADIATION SAFETY ASSOCIATES


19 Pendleton Drive
Hebron, CT 06248
(860) 228-0487

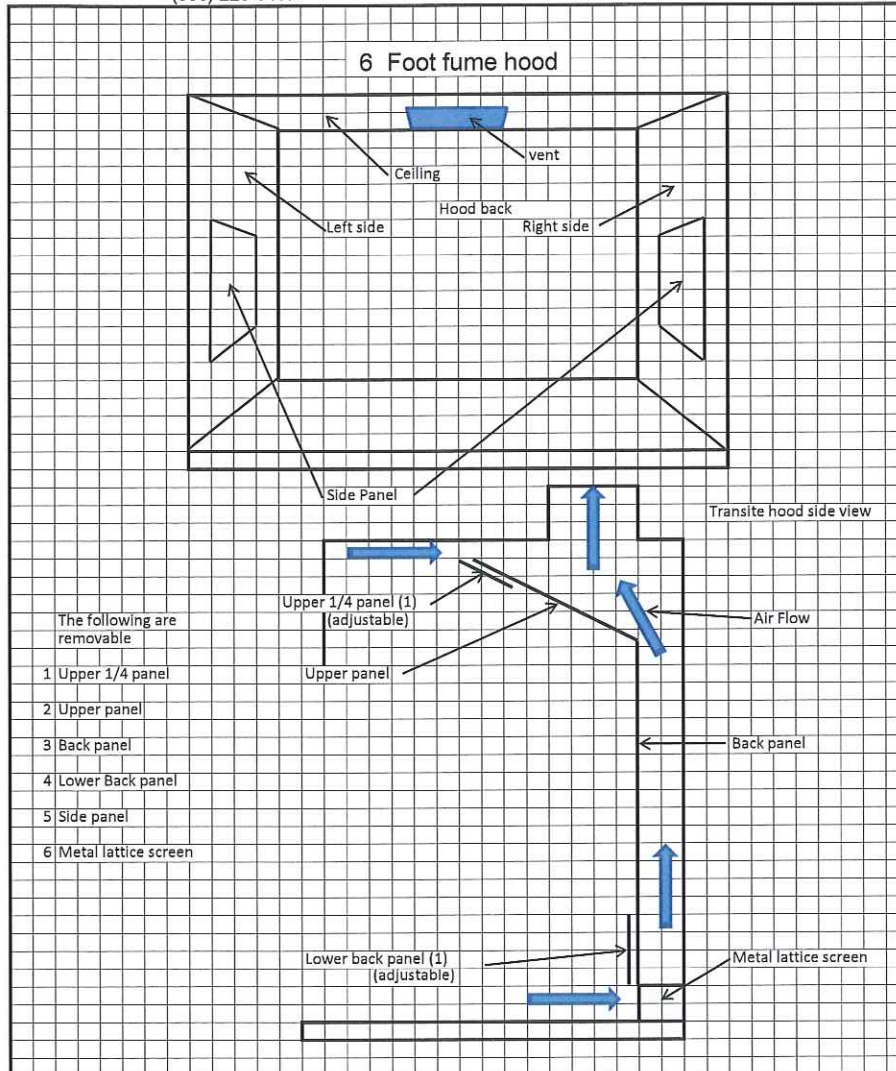

x

RADIATION SAFETY ASSOCIATES

19 Pendleton Drive
 Hebron, CT 06248
 (860) 228-0487



RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **2/18/2011**Date Counted: **2/18/2011**Customer: **Chemtura**Location: **1202 Hood A 8'**Project: **Lab Decommissioning**Samp. Description: **Survey Wipes**Matrix: **Wipes****C-14 LLD dpm= 44.57**

RSA ID#	CUST. ID#	Location			C-14 CPM	C-14 DPM	
BG		BACKGROUND			43.60		
1		Left Side			23.90	26.10	
2		Left Back Front			10.70	11.80	
3		Left Back Back			12.10	13.10	
4		Right Back Front			17.30	18.60	
5		Right Back Back			7.30	8.00	
6		Right Side			16.50	18.40	
7		Left Counter			11.80	13.20	
8		Right Counter			30.40	34.10	
9		Sill			1.70	1.90	
10		Upper Pannel Left Front			25.30	28.40	
11		Upper Pannel Left Back			24.90	27.80	
12		Upper Pannel Right Front			9.90	11.10	
13		Upper Pannel Right Back			28.90	32.50	
14		Left Cover			20.40	22.80	
15		Right Cover			9.20	10.30	
16		Hood Back Upper Left			0.00	0.00	
17		Hood Back Upper Right			24.50	27.90	
18		Hood Back Lower Left			15.30	17.20	
19		Hood Back Lower Right			20.10	22.60	
20		Glass Left			32.60	36.50	
21		Glass Right			47.30	52.80	
22		Ceiling Left			28.30	32.10	
23		Ceiling Right			27.30	31.20	
C-14		QC - C-14			124232.40	134276.30	
BL		QC Blank			16.80	18.20	

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **2/18/2011**Date Counted: **2/18/2011**Customer: **Chemtura**Location: **1202 Hood B 6'**Project: **Lab Decommissioning**Samp. Description: **Survey Wipes**Matrix: **Wipes****C-14 LLD dpm= 43.14**

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq	
	BG	BACKGROUND			40.60		
1		Left Side			22.10	24.10	
2		Hood Back Upper Left			12.80	13.80	
3		Hood Back Upper Right			66.20	71.70	
4		Hood Back Lower Left			0.00	0.00	
5		Hood Back Lower Right			62.80	67.90	
6		Right Side			13.80	14.90	
7		Left Counter			20.30	21.90	
8		Right Counter			23.50	25.40	
9		Sill			11.30	12.30	
10		Left Cover			15.90	17.10	
11		Right Cover			3.30	3.60	
12		Left Glass			20.90	22.50	
13		Right Glass			0.00	0.00	
14		Lower Back Front			16.30	17.70	
15		Lower Back Back			6.50	7.10	
16		Upper 1/4 Fron			16.10	17.60	
17		Upper 1/4 Back			19.10	20.70	
18		Screen			20.60	22.70	
19		Left Ceiling			3.70	4.10	
20		Right Ceiling			28.40	30.80	
C-14		QC C-14			117684.00	133716.60	
BL		QC Blank			11.60	12.60	

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer **Chemtura**Customer Samp No. **N/A**Location: **1202 Hood C 6'**RSA Lab Sample No. **N/A**Project: **Lab Decommissioning**Date Collected: **2/18/2011**Samp. Description: **Survey Wipes**Date Counted: **2/18/2011**Matrix: **Wipes****C-14 LLD dpm= 40.98**


RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq	
BG		BACKGROUND			36.30		
1		Left Side			11.90	12.90	
2		Back Left Front			11.20	12.10	
3		Back Right Front			12.80	13.80	
4		Right Side			16.40	17.70	
5		Left Counter			10.00	10.90	
6		Right Counter			8.70	9.50	
7		Sill			1.00	1.10	
8		Lower Back Fron			5.70	6.10	
9		Lower Back Back			68.90	74.40	
10		Upper Pannel Front			0.00	0.00	
11		Upper Pannel Back			15.40	16.60	
12		Upper 1/4 Front			4.30	4.60	
13		Upper 1/4 Back			12.30	13.40	
14		Glass Left			16.80	18.10	
15		Glass Right			0.50	0.50	
16		Back Pannel Left Back			7.20	7.90	
17		Back Pannel Right Back			11.20	12.10	
18		Left Cover			16.80	18.20	
19		Right Cover			5.40	5.80	
20		Hood Back Upper Left			17.30	18.70	
21		Hood Back Upper Right			18.30	19.80	
22		Hood Back Lower Left			11.10	12.10	
23		Hood Back Lower Right			11.30	12.20	
C-14		QC C-14			121657.00	134397.90	
24		Ceiling Left			17.90	19.40	
25		Ceiling Right			14.40	15.60	
BL		QC Blank			11.60	12.60	

Room 1203 Scoping Survey

Contents


Page

- 2 Floor Plan
- 3 Drawing of a typical 6-foot fume hood
- 4 Wipe test data for Hood 68
- 5 Wipe test data for Hood 65




19 Pendleton Drive
Hebron, CT 06248
(860) 228-0487

6 Foot fume hood

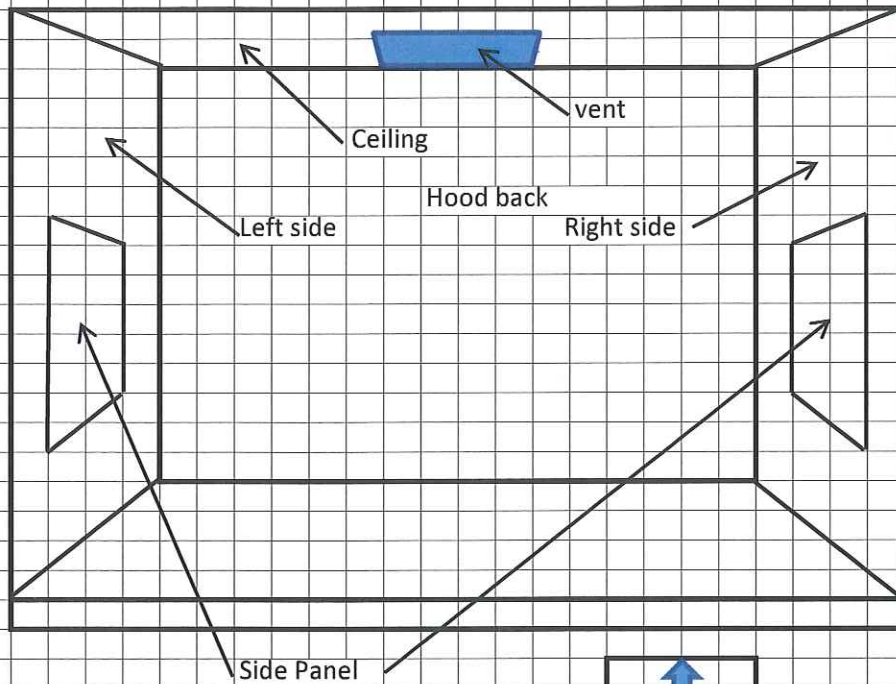

Transite hood side view



The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 2

Report No. N/A

Customer Samp No. N/A

RSA Lab Sample No. N/A

Date Collected: 3/9/2011

Date Counted: 3/10/2011

Customer: Chemtura

Location: 1203 Hood 68

Project: Lab Decommissioning

Samp. Description: Survey Wipes

Matrix: Wipes

C-14 LLD dpm= 43.09

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
BG		BACKGROUND			40.50	
1		Left Side			8.60	9.50
2		Hood Back Left Upper			2.50	2.80
3		Hood Back Right Upper			12.90	14.30
4		Hood Back Left Lower			10.70	11.80
5		Hood Back Right Lower			15.00	16.60
6		Right Side			17.50	19.30
7		Counter L			7.10	7.80
8		Counter R			88.60	97.40
9		Sill			104.90	116.50
10		Ceiling Left			9.20	10.20
11		Ceiling Right			19.30	21.60
12		Glass Left			18.20	20.20
13		Glass Right			16.20	18.00
14		Screen			14.10	15.80
15		Left Side Cover - front			7.10	7.80
16		Right Side Cover - front			4.50	4.90
17		Left Side Cover - back			12.50	13.89
18		Upper Panel Left Front			5.20	5.00
19		Upper Panel Left Back			3.50	3.90
20		Upper Panel Right Front			14.80	16.40
21		Upper Panel Right Back			3.60	4.00
22		Lower back Panel Left Front			14.50	16.00
23		Lower back Panel Left Back			12.30	13.70
C-14		QC C-14			120857.10	133455.30
24		Lower back Panel Right Front			19.70	21.70
25		Lower back Panel Right Back			9.40	10.50
26		EMPTY VIAL				
27		Upper 1/4 panel Left Front			33.80	37.40
28		Upper 1/4 panel Left Back			21.90	24.30
29		Upper 1/4 panel Right Front			11.80	13.10
30		Upper 1/4 panel Right Back			9.00	10.00
31		Back Panel Left Front			7.50	8.20
32		Back Panel Left Back			11.00	12.10
33		Back Panel Right Front			16.20	18.00
34		Back Panel Right Back			11.30	12.50
BL		QC Blank			11.10	12.10

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **3/9/2011**Date Counted: **3/10/2011**Customer: **Chemtura**Location: **1203 Hood 65**Project: **Lab Decommissioning**Samp. Description: **Survey Wipes**Matrix: **Wipes****C-14 LLD dpm= 41.04**


RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
	BG	BACKGROUND			36.40	
1		Left Side			15.90	17.40
2		Hood Back Left Upper			20.10	22.20
3		Hood Back Right Upper			15.20	16.80
4		Hood Back Left Lower			14.20	15.70
5		Hood Back Right Lower			15.50	17.20
6		Right Side			7.00	7.70
7		Counter Left			0.00	0.00
8		Counter Right			13.60	15.20
9		Sill			2.60	3.00
10		Ceiling Left			16.90	18.80
11		Ceiling Right			23.30	26.00
12		Glass Left			7.10	7.80
13		Glass Right			9.00	9.90
14		Screen			13.90	15.50
15		Left Cover			6.60	7.20
16		Right Cover			0.00	0.00
17		Upper Panel Left Front			14.50	16.00
18		Upper Panel Left Back			0.00	0.00
19		Upper Panel Right Front			10.80	11.90
20		Upper Panel Right Back			17.10	19.00
21		Lower Back Front			14.10	15.60
22		Lower Back Back			29.60	32.90
23		Upper 1/4 Panel Front			32.80	36.40
C14		QC C-14			125638.30	135986.90
24		Upper 1/4 Panel Back			21.00	23.40
BL		Blank			37.80	41.10

Room 1204 Scoping Survey

Contents


Page

- 2 Floor Plan
- 3 Drawing of a typical 6-foot fume hood
- 4 Wipe test data for Hood 62
- 5 Wipe test data for Hood 53




19 Pendleton Drive
Hebron, CT 06248
(860) 228-0487

6 Foot fume hood



Transite hood side view

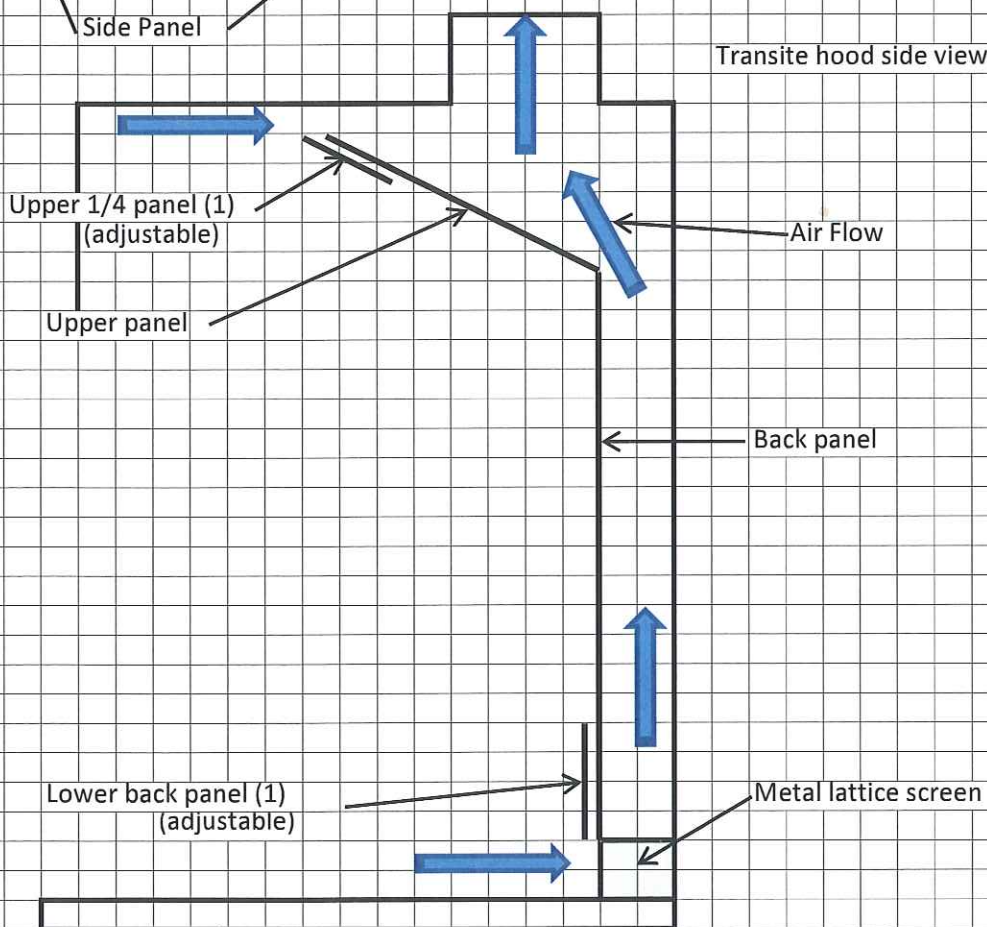

The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **2/18/2011**Date Counted: **2/18/2011**Customer: **Chemtura**Location: **1204 Hood 62**Project: **Lab Decommissioning**Samp. Description: **Survey wipes**Matrix: **Wipes****C-14 LLD dpm= 43.14**

RSA ID#	CUST. ID#	Location			C-14 CPM	C-14 DPM	
BG		BACKGROUND			40.60		
1		Left Side			47.20	52.80	
2		Hood Back Upper Left			23.20	26.10	
3		Hood Back Upper Right			66.10	75.00	
4		Hood Back Lower Left			216.30	243.00	
5		Hood Back Lower Right			11.80	13.20	
6		Right Side			15.80	17.60	
7		Left Countertop			25.30	28.40	
8		Right Countertop			23.80	26.70	
9		Sill			7.40	8.40	
10		Lower Back Panel Front			5.20	5.80	
11		Lower Back Panel Back			226.90	255.10	
12		Glass Left			11.60	13.00	
13		Glass Right			27.00	30.30	
14		Left Cover			15.70	17.60	
15		Right Cover			12.80	14.20	
16		Upper Panel Front			36.90	41.30	
17		Upper Panel Back			49.70	55.80	
18		Upper Panel 1/4 Front			26.10	29.10	
19		Upper Panel 1/4 Back			43.90	49.20	
20		Left Ceiling			21.10	23.70	
21		Right Ceiling			10.20	11.50	
22		Screen			28.40	32.20	
C-14		QC C-14			118209.60	134604.40	
BL		QC Blank			0.00	0.00	

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **2/28/2011**Date Counted: **2/28/2011**Customer: **Chemtura**Location: **1204 Hood 53**Project: **Lab Decommissioning**Samp. Description: **Survey wipes**Matrix: **Wipes****C-14 LLD dpm= 35.60**


RSA ID#	CUST. ID#	Location			C-14 CPM	C-14 DPM
BG		BACKGROUND			26.60	
1		Left Side			39.00	43.70
2		Back Upper Left			62.00	69.50
3		Back Upper Right			43.10	48.30
4		Back Lower Left			13.60	15.30
5		Back Lower Right			73.40	82.70
6		Right Side			26.20	29.30
7		Counter Left			19.90	22.60
8		Counter Right			95.30	107.90
9		Sill			30.60	34.30
10		Upper 1/4 Front			24.90	27.80
11		Upper 1/4 Back			63.30	71.10
12		Ceiling Left			16.30	18.30
13		Ceiling Right			46.00	51.80
14		Vent			145.80	176.00
15		Glass Left			13.90	15.60
16		Glass Right			18.10	20.20
17		Screen			43.20	48.60
18		Right Cover			27.90	31.30
C-14		QC C-14			120208.50	132827.10
BL		QC Blank			9.50	10.30

Room 1205 Scoping Survey

Contents


Page

2	Floor Plan
3	Drawing of a typical 6-foot fume hood
4	Wipe test data for Hood 50
5	List of objects surveyed
6-8	Object wipe results
9	List of additional objects surveyed
10-11	Additional object wipe results




Floor Plan Room 1205

19 Pendleton Drive
Hebron, CT 06248
(860) 228-0487



Transite hood side view



The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 29

Report No. **N/A**Customer: **Chemtura**Customer Samp No. **N/A**Location: **1205 Hood 50**RSA Lab Sample No. **N/A**Project: **Lab Decommissioning**Date Collected: **2/15/2011**Samp. Description: **Wipes**Date Counted: **2/15/2011**Matrix: **Wipes****C-14 LLD dpm= 37.07**

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
BG		BACKGROUND			29.10	
1		Left Side			2.60	2.80
2		Right Side			10.50	11.40
3		Left Lower Back Front			15.80	17.00
4		Left Lower Back Back			12.30	13.20
5		Right Lower Back Front			12.80	13.80
6		Right Lower Back Back			28.90	31.20
7		Left Upper 1/4 Front			4.60	5.00
8		Left Upper 1/4 Back			14.70	15.90
9		Right Upper 1/4 Front			15.30	16.60
10		Right Upper 1/4 Back			18.40	19.80
11		Ring Stand			3.00	3.30
12		Ring Stand			13.30	14.40
13		Ring Stand			15.00	16.30
14		Screen			9.40	10.20
15		Glass Left Back			15.80	17.00
16		Glass Right Back			13.90	15.00
17		Counter Left			12.00	13.00
18		Counter Right			13.70	14.80
19		Sill			10.60	11.50
20		Hood Back Left Upper			36.40	39.30
21		Hood Back Right Upper			14.10	15.30
22		Hood Back Left Lower			19.50	21.00
23		Hood Back Right Lower			14.60	15.80
C-14		QC C-14			122063.50	134951.40
BL		QC Blank			19.30	21.00

Object #	Description
1	Organization
2	Rotavapor R11G
3	Plexiglass Shield
4	Dell Computer PC-506
5	Cartridge 5415D
6	HPLC Radmonitor LB507A
7	Dionex UVD170U UV-40
8	UC100 Chromatograph Interface
9	Beckman LSC Computer
10	Beckman Printer
11	Beckman LSC
12	Fisher Isotemp 500 Oven
13	Fisher FS60 H Water Bath
14	Boekel Dessicator
15	Boekel Dessicator
16	Rotary Shaker Model G2
17	Blender Base
18	Power Supply
19	Vortex Genie 2
20	Automixer
21	Hot Plate
22	Vortex Genie 2
23	HP Printer
24	Amdek Monitor
25	Link Monitor
26	Power Supply
27	Phone
29	Balance
30	Phone
31	Filing Cabinet
32	Filing Cabinet
33	Wood Table
65	Freezer FR-02
66	Refrigerator RF25A/B
67	Environmental Chamber EV-07
68	Refrigerator RF-21
69	Flammables Locker
297	Plexiglass Shield

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 3

Report No. **N/A**Customer: **Chemtura**Customer Samp No. **N/A**Location: **1205 Objects**RSA Lab Sample No. **N/A**Project: **Lab Decommissioning**Date Collected: **01/31/11 - 02/14/11**Samp. Description: **Wipes**Date Counted: **01/31/11 - 02/14/11**Matrix: **Wipes****C-14 LLD dpm= 38.20**

RSA ID#	CUST. ID#	Location	0 CPM	0 DPM	C-14 CPM	dpm/100 cm sq
BG		BACKGROUND			31.10	
1		Object 1			1.50	1.70
2		Object 2			15.70	17.20
3		Object 3			10.80	11.80
4		Object 4			20.30	22.20
5		Object 5			14.20	15.50
6		Object 6			13.30	14.50
7		Object 7			23.50	25.60
8		Object 8			14.30	15.60
9		Object 9			9.50	10.40
10		Object 10			11.10	12.10
11		Object 11			8.80	9.60
12		Object 11			31.30	34.40
13		Object 12			16.00	17.40
14		Object 12			11.90	13.00
15		Object 13			24.60	26.90
16		Object 14			12.10	13.20
17		Object 15			26.30	28.90
18		Object 16			0.90	1.00
19		Object 17			16.20	17.70
20		Object 18			11.00	12.00
21		Object 19			12.60	13.70
22		Object 20			26.10	28.50
23		Object 21			20.70	22.50
C14		QC C-14			121074.60	133798.90
24		Object 22			19.40	21.20
25		Object 23			19.90	21.80
26		Object 24			0.10	0.10
27		Object 25			19.40	21.20
28		Object 26			24.00	26.30
29		Object 27			19.80	21.70
30		Object 29			3.60	3.90
31		Object 30			5.80	6.30
32		Object 31			10.20	11.30
33		Object 32			6.10	6.70
34		Object 33			14.30	15.70

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 2 of 3

RSA ID#	CUST. ID#	LOCATION	0 CPM	0 DPM	C-14 CPM	dpm/100 cm sq
35		Object 67 Front			6.10	6.60
36		Object 67 Right Side			14.90	16.20
37		Object 67 Left Side			10.60	11.50
38		Object 67 Inside Right			6.40	6.90
39		Object 67 Inside Left			18.10	19.70
40		Object 67 Back			6.70	7.30
41		Object 67 Bottom			19.10	20.90
42		Object 67 Inside Door			15.40	16.90
43		Object 68 Top			5.80	6.30
44		Object 68 Left Side			19.60	21.30
45		Object 68 Right Side			13.40	14.60
46		Object 68 Front			15.60	17.00
BL		QC Blank			9.90	10.70
47		Object 68 Inside Left			16.40	17.80
48		Object 68 Back			14.00	15.40
49		Object 68 Inside Right			19.40	21.20
50		Object 68 Bottom			27.60	30.30
51		Object 68 Inside Door			10.40	11.70
52		Object 69 Top			14.10	15.40
53		Object 69 Left Side			6.20	6.80
54		Object 69 Right Side			9.60	10.50
55		Object 69 Front			18.40	20.00
56		Object 69 Inside Left			14.00	15.30
57		Object 69 Shelf			55.20	60.30
58		Object 69 Inside Right			12.80	13.90
59		Object 69 Bottom			14.70	16.10
60		Object 69 Inside Door			20.20	22.00
61		Object 297			9.20	10.10
62		Object 65 Top			37.90	41.00
63		Object 65 R Side			17.10	18.40
64		Object 65 L Side			31.00	33.40
65		Object 65 Door Front			16.10	17.40
66		Object 65 Inside L			7.00	7.60
67		Object 65 Inside Back			38.50	41.40
68		Object 65 Inside R			28.10	30.20
69		Object 65 Bottom			120.50	130.50
70		Object 65 Inside Door			170.60	184.30
71		Object 66 Top			19.80	21.60
72		Object 66 R Side			11.90	12.90
73		Object 66 L Side			8.20	8.80
74		Object 66 Door Front			25.90	27.90
75		Object 66 Freezer Inside L			3.70	4.00
76		Object 66 Freezer Inside Back			12.90	13.90

Page 3 of 3

[illegible]

Chemtura Middlebury

Object # Description

339 Hot Plate
340 Blender
341 Blender
342 Stir Plate
344 Blender
345 Hot plate
346 Water Bath
347 Hot Plate
348 Glass Blender w/o Base
349 Metal Blender w/o Base
350 Rheostat
351 Stirrer
352 Stirrer
353 Label Printer
354 Rheostat
355 Electric Controller
356 Large Sorval Rotor
357 Vial Heater
358 Harvard Apparatus
359 Rheostat
360 UPS
361 Rheostat
362 Hot Plate
363 Column Heater
364 Rheostat
365 UPS
366 UPS
367 UPS
368 Small Sorval Rotor
369 UPS
370 Hot Plate
371 Vortex Mixer
372 Fisher Sci Mixer
373 Stirrer
374 Rheostat
375 Alltech Heater
376 Polytron
377 Blender base
378 Hot Plate
379 Large Metal Blender w/o Base

Object # Description

380 Stirrer
381 Hot Plate
382 Large Blender w/o Base
383 Shimadzu Degasser
384 Rheostat
385 Hot Plate
386 Hot Plate
387 Blender Base
388 Stirrer
389 Stirrer
390 Rotavapor Head
391 Hot Plate
392 Rheostat
393 Blok Heater
394 Vortex Mixer
395 Tire Clock
396 Rheostat
397 Vortex Mixer
398 Rotavapor Unit
399 P580 Pump PM-62
400 Dessicator
401 Power Strip

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 2

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **2/14/2011**Date Counted: **2/14/2011**Customer: **Chemtura**Location: **1205 Additional Objects**Project: **Lab Decommissioning**Samp. Description: **Survey Wipes**Matrix: **Wipes****C-14 LLD dpm= 43.57**

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
BG		BACKGROUND			41.50	
1		Object 339			13.80	25.70
2		Object 340			13.60	14.60
3		Object 341			37.10	40.10
4		Object 342			38.70	42.00
5		Object 344			13.50	14.60
6		Object 345			21.30	23.00
7		Object 346			27.30	29.60
8		Object 347			17.20	18.60
9		Object 348			17.80	19.20
10		Object 349			8.20	8.90
11		Object 350			16.50	17.80
12		Object 351			24.10	25.90
13		Object 352			12.00	13.00
14		Object 353			18.00	19.40
15		Object 354			10.00	10.80
16		Object 355			19.00	20.50
17		Object 356			16.60	17.90
18		Object 357			15.60	16.80
19		Object 358			13.40	14.50
20		Object 359			8.40	9.10
21		Object 360			13.30	14.30
22		Object 361			19.20	20.70
23		Object 362			11.50	12.40
C-14		QC C-14			121659.70	134504.90
24		Object 363			9.90	10.70
25		Object 364			18.70	20.10
26		Object 365			15.40	16.70
27		Object 366			29.30	31.80
28		Object 367			17.60	19.00
29		Object 368			14.80	16.00
30		Object 369			11.90	12.80
31		Object 370			412.60	445.20
32		Object 371			122.90	133.30
33		Object 372			107.50	116.10
34		Object 373			53.30	57.40

Page 2 of 2


11

Room 1206 Scoping Survey

Contents


Page

2	Floor Plan
3	Drawing of a typical 6-foot fume hood
4	Wipe test data for Hood 48
5	Wipe test data for Hood 51
6	List of objects surveyed
7-8	Object wipe results




Room 1206 Scoping Survey
19 Pendleton Drive
Hebron, CT 06248
(860) 228-0487

6 Foot fume hood

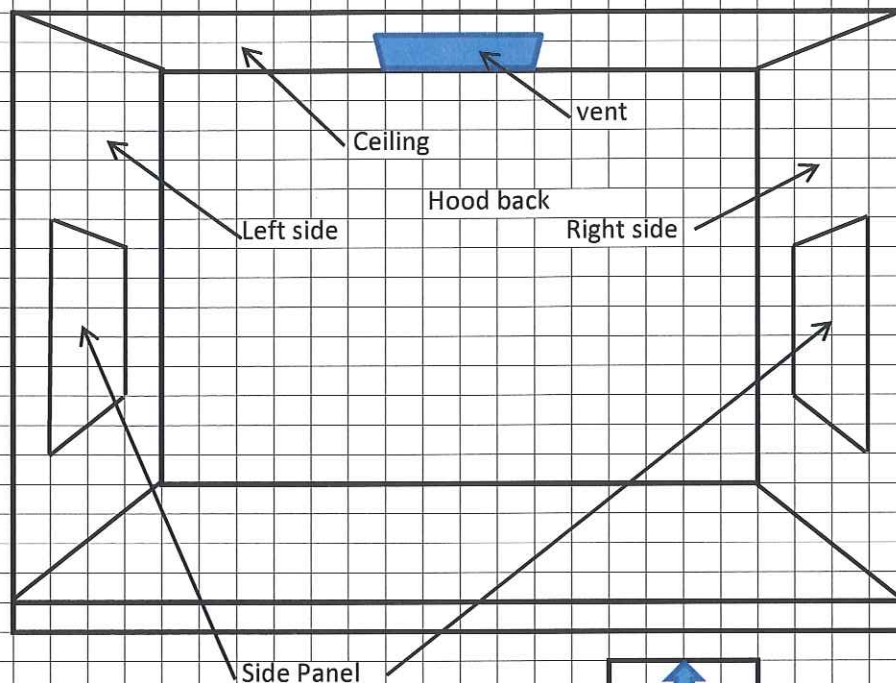

Transite hood side view

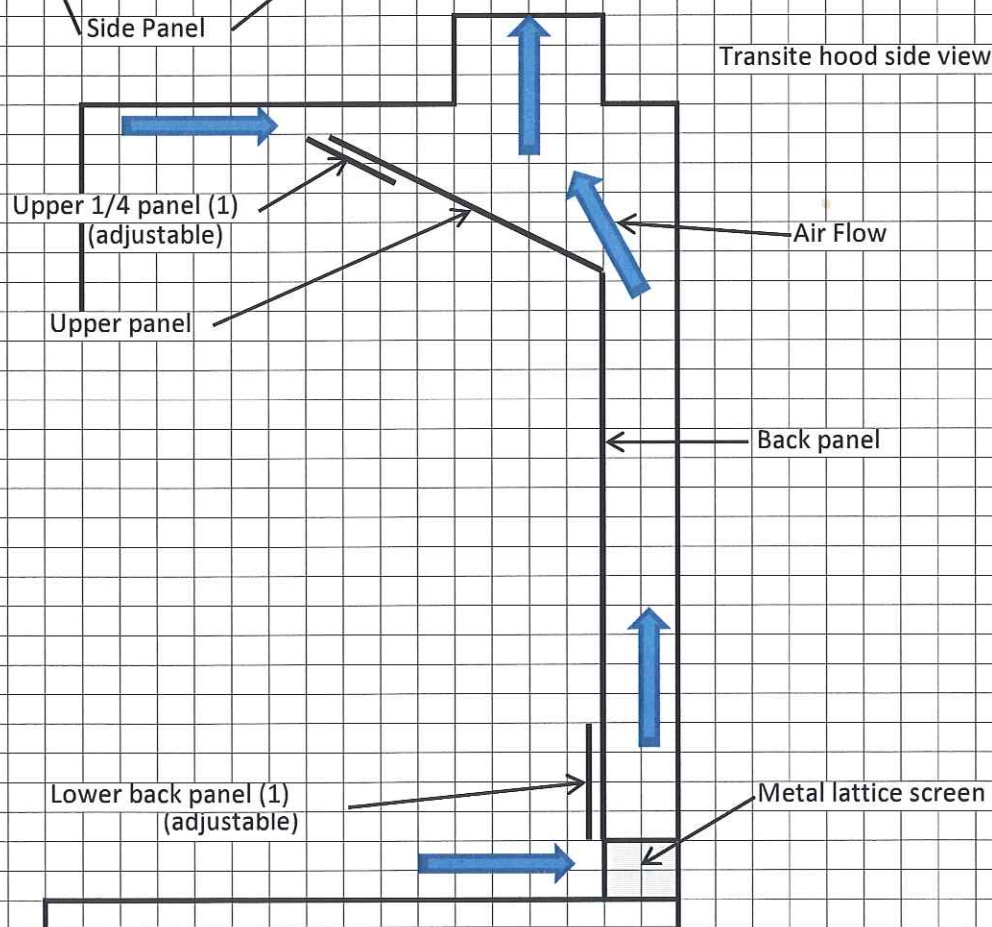

The following are removable

- 1 Upper 1/4 panel
- 2 Upper panel
- 3 Back panel
- 4 Lower Back panel
- 5 Side panel
- 6 Metal lattice screen

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 1

Report No. **N/A**Customer: **Chemtura**Customer Samp No. **N/A**Location: **1206 Hood 48**RSA Lab Sample No. **N/A**Project: **Lab Decommissioning**Date Collected: **3/14/2011**Samp. Description: **Wipes**Date Counted: **3/14/2011**Matrix: **Wipes****H-3 LLD dpm= 43.70****C-14 LLD dpm= 43.09**

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
BG		BACKGROUND			40.50	
1		Lside			1.20	1.30
2		Hood Back Upper Left			19.50	21.40
3		Hood Back Upper Right			5.00	5.50
4		Hood Back Lower Left			13.60	15.00
5		Hood Back Lower Right			33.00	36.80
6		Hood Right Side			24.70	27.30
7		Counter Left			33.50	36.90
8		Counter Right			58.30	64.40
9		Sill			14.90	16.40
10		Ceiling Left			19.00	21.00
11		Ceiling Right			12.70	14.20
12		Glass Left			14.40	15.90
13		Glass Right			4.00	4.40
14		Screen			33.50	37.90
15		Back Botton Left Front			25.80	28.60
16		Back Botton Left Back			9.60	10.60
17		Back Botton Right Front			12.60	13.90
18		Back Botton Right Back			5.60	6.10
19		Left Cover			24.30	26.80
20		Right Cover			10.10	11.10
21		Back Upper 1/4 Panel Left Front			17.00	18.70
22		Back Upper 1/4 Panel Left Back			22.50	24.90
23		Back Upper 1/4 Panel Right Front			15.80	17.50
C-14		QC C-14			114821.60	134640.70
24		Back Upper 1/4 Panel Right Back			39.70	43.80
BL		QC Blank			14.40	15.80

Page 1 of 1

Customer: **Chemtura**

Location: 1206 Hood 51

Project: **Lab Decommissioning**

Samp. Description: **Wipes**

Matrix: **Wipes**

[illegible]

Object #	Description
35	Rotavator & Bath
36	Water Bath
37	Mettler A30 Balance
38	Mettler PM4600 Balance
39	Rotavator I M
40	Blender Base
41	Power Supply
42	Hot Plate
43	Hitachi SCM-03
44	HPLC Pump
45	HPLC Pump
46	Retriever II
47	Plexiglass Shield
48	Beta -RAM
49	HPLC Pump P580
50	Dell Computer & Monitor
51	UV Detector UVD170U
52	HPLC Pump
53	HPLC
54	SE 120 Plotter
56	Retriever II
57	Table
58	Table
59	Evaporator
60	HP Printer
61	Desktop Computer
62	Label Printer
63	HP Desk Jet
64	Phone
70	Refrigerator RF -19 A/B Diagram
71	Environmental Chamber EV -05 Diagram
72	Freezer FR-06 Diagram
319	Filing Cabinet
320	Filing Cabinet
321	Vortex Mixer
322	Sonicator

RSA Laboratories
A Division of Radiation Safety Associates
Radiochemistry Analysis Data Sheet

Page 1 of 2

Report No. **N/A**Customer Samp No. **N/A**RSA Lab Sample No. **N/A**Date Collected: **02/02/11 - 02/09/11**Date Counted: **02/02/11 - 02/09/11**Customer: **Chemtura**Location: **1206 Objects**Project: **Lab Decommissioning**Samp. Description: **Wipes**Matrix: **Wipes****C-14 LLD dpm= 40.47**

RSA ID#	CUST. ID#	Location			C-14 CPM	dpm/100 cm sq
	BG	BACKGROUND			35.30	
1		Object 35			22.50	24.30
2		Object 36			25.40	27.50
3		Object 37			10.30	11.50
4		Object 38			19.10	20.70
5		Object 39			15.10	16.40
6		Object 40			20.70	22.40
7		Object 41			14.90	16.10
8		Object 42			44.00	47.50
9		Object 43			0.00	0.00
10		Object 44			3.30	3.50
11		Object 45			2.30	2.50
12		Object 46			18.40	19.90
13		Object 47			2.80	3.00
14		Object 48			8.70	9.40
15		Object 49			5.10	5.50
16		Object 50			21.10	22.90
17		Object 51			22.70	24.50
18		Object 52			25.00	27.00
19		Object 53			27.40	29.60
20		Object 54			26.60	28.90
21		Object 56			27.40	29.70
22		Object 57			18.80	20.30
23		Object 58			15.20	164.00
C14		QC C-14			12125.00	133918.70
24		Object 59			23.40	25.50
25		Object 60			55.50	60.10
26		Object 61			19.30	20.90
27		Object 62			29.60	32.00
28		Object 63			12.00	13.00
29		Object 64			20.10	21.70
30		Object 70 Top			24.10	26.10
31		Object 70 Right Side			18.30	19.70
32		Object 70 Left Side			14.50	15.60
33		Object 70 Front			14.10	15.60
34		Object 70 Left Inside Freezer			25.40	27.30

RSA Laboratories					
A Division of Radiation Safety Associates					
Radiochemistry Analysis Data Sheet					
		Page 2 of 2			
	CUST.	LOCATION		C-14	dpm/100 cm sq
RSA ID#	ID#			CPM	
35		Object 70 Back Freezer		18.3	19.7
36		Object 70 Right Inside Freezer		25.2	27.2
37		Object 70 Bottom Freezer		27.8	30
38		Object 70 Left Inside Fridge		17.9	19.3
39		Object 70 Back Fridge		14.5	15.6
40		Object 70 Right Inside Frige		6.9	7.4
41		Object 70 Bottom Frige		13.1	14.1
42		Object 70 Inside Door Freezer		19.1	20.7
43		Object 70 Inside Door Frige		1.7	1.8
44		Object 71 Top		0	0
45		Object 71 Right Side		10.2	11
46		Object 71 Left Side		10.4	11.2
BL		QC Blank		10.3	11.2
47		Object 71 Front		13	14
48		Object 71 Left Inside		26.1	28.1
49		Object 71 Back		6.9	7.5
50		Object 71 Right Inside		19.6	21.1
51		Object 71 Bottom		21.5	23.1
52		Object 71 Inside Door		24.4	26.4
53		Object 72 Top		10.6	11.4
54		Object 72 Right Side		22.7	24.4
55		Object 72 Left Side		9.4	10.1
56		Object 72 Front		13.3	14.3
57		Object 72 Left Inside		21.9	23.6
58		Object 72 Back		68.2	73.7
59		Object 72 Right Inside		34.6	37.3
60		Object 72 Bottom		165.5	179.9
61		Object 72 Inside Door		161	174
62		Object 319		11.4	12.3
63		Object 320		14.3	15.5
64		Object 321		47.5	51.2
65		Object 322		19.2	20.8
66		Object 72 Right Side Upper er post decon rewipe		71.1	76.5
67		Object 72 Right Side Lower er post decon rewipe		64.3	69.2
68		Object 72 Bottom Right post decon rewipe		354.2	382.5
69		Object 72 Bottom Left post decon rewipe **		4219.8	4563.4
			** Disposed as rad waste		