

North East Technical Services, Inc.

75 Aileron Ct., Suite 4

Westminster, MD 21157

Ph: 410.751.5090 Fax: 410.751.5091

Infrared Analyzers

65 Lyman Drive

Williston, VT 05495

ATTN: JP Philipss

Shipping Address: 65 Lyman Drive

Williston, VT 05495

LEAK TEST CERTIFICATE

MD Materials License # MD-13-020-01

This certifies that leak test analysis was conducted on the sample with the following information. The results shown below accurately represent the level of removeable contamination.

Gauge Model 3216 **Gauge S/N** R150 **Leak Test Date** 10/10/2013

Source

Reading in microCuries

47-5743


0.00000

Note: 0.005 microCuries (185 Bq) or greater is considered a leaking source. The source(s) tested above may remain in use.

Reviewed by: Douglas Simes

Date: OCT 16 2013

Monday, October 21, 2013

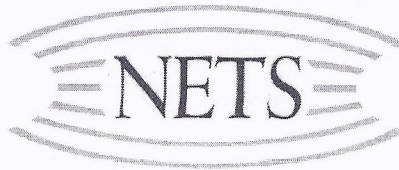

North East Technical Services, Inc.

75 Aileron Ct., Suite 4

Westminster, MD 21157

Ph: 410.751.5090 Fax: 410.751.5091

Infrared Analyzers

65 Lyman Drive

Williston, VT 05495

ATTN: JP Philipss

Shipping Address: 65 Lyman Drive

Williston, VT 05495

LEAK TEST CERTIFICATE

MD Materials License # MD-13-020-01

This certifies that leak test analysis was conducted on the sample with the following information. The results shown below accurately represent the level of removeable contamination.

Gauge Model	3216	Gauge S/N	R501	Leak Test Date	10/10/2013
Source		Reading in microCuries			
	47-746	0.00000			

Note: 0.005 microCuries (185 Bq) or greater is considered a leaking source. The source(s) tested above may remain in use.

Reviewed by: Don L. Sims

Date: OCT 16 2013

Monday, October 21, 2013



North East Technical Services, Inc.

75 Aileron Ct., Suite 4

Westminster, MD 21157

Ph: 410.751.5090 Fax: 410.751.5091

Infrared Analyzers

65 Lyman Drive

Williston, VT 05495

ATTN: JP Philipss

Shipping Address: 65 Lyman Drive

Williston, VT 05495

LEAK TEST CERTIFICATE

MD Materials License # MD-13-020-01

This certifies that leak test analysis was conducted on the sample with the following information. The results shown below accurately represent the level of removeable contamination.

Gauge Model	3216	Gauge S/N	R273	Leak Test Date	10/10/2013
--------------------	-------------	------------------	-------------	-----------------------	-------------------

Source	Reading in microCuries
---------------	-------------------------------

47-9174	0.00000
---------	---------

Note: 0.005 microCuries (185 Bq) or greater is considered a leaking source. The source(s) tested above may remain in use.

I Reviewed by: *Douglas Simes*

Date: OCT 16 2013

Monday, October 21, 2013



North East Technical Services, Inc.

75 Aileron Ct., Suite 4

Westminster, MD 21157

Ph: 410.751.5090 Fax: 410.751.5091

Infrared Analyzers

65 Lyman Drive

Williston, VT 05495

ATTN: JP Philipss

Shipping Address: 65 Lyman Drive

Williston, VT 05495

LEAK TEST CERTIFICATE

MD Materials License # MD-13-020-01

This certifies that leak test analysis was conducted on the sample with the following information. The results shown below accurately represent the level of removeable contamination.

Gauge Model 3216 Gauge S/N R238 Leak Test Date 10/14/2013

Source

Reading in microCuries


0.00008236

Note: 0.005 microCuries (185 Bq) or greater is considered a leaking source. The source(s) tested above may remain in use.

I *signed by:* *Douglas Sime*

Date: OCT 22 2013

Thursday, October 24, 2013

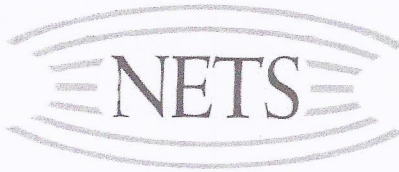

North East Technical Services, Inc.

75 Aileron Ct., Suite 4

Westminster, MD 21157

Ph: 410.751.5090 Fax: 410.751.5091

Infrared Analyzers

65 Lyman Drive

Williston, VT 05495

ATTN: JP Philipss

Shipping Address: 65 Lyman Drive

Williston, VT 05495

LEAK TEST CERTIFICATE

MD Materials License # MD-13-020-01

This certifies that leak test analysis was conducted on the sample with the following information. The results shown below accurately represent the level of removeable contamination.

Gauge Model	3216	Gauge S/N	R53	Leak Test Date	10/14/2013
--------------------	-------------	------------------	------------	-----------------------	-------------------

Source

Reading in microCuries

0.00008236

Note: 0.005 microCuries (185 Bq) or greater is considered a leaking source. The source(s) tested above may remain in use.

I  **owed by:** _____

Date: OCT 22 2013

Thursday, October 24, 2013