

RI - DNMS Licensee Event Report Disposition

Licensee:	Agilent Technologies				
Event Description:	Loss of Licensed Material				
License No:	07-28762-01	Docket No:	03032742	MLER-RI:	2017-001
Event Date:	11/07/16	Report Date:	12/07/16	HQ Ops Event #:	52410

1. REPORTING REQUIREMENT

<input type="checkbox"/>	10 CFR 20.1906 Package Contamination	<input type="checkbox"/>	10 CFR 30.50 Report
<input checked="" type="checkbox"/>	10 CFR 20.2201 Theft or Loss	<input type="checkbox"/>	10 CFR 35.3045 Medical Event
<input type="checkbox"/>	10 CFR 20.2203 30 Day Report	<input type="checkbox"/>	License Condition
<input type="checkbox"/>	Other		

2. REGION I RESPONSE

<input type="checkbox"/>	Immediate Site Inspection	Inspector/Date	
<input type="checkbox"/>	Special Inspection	Inspector/Date	
<input type="checkbox"/>	Telephone Inquiry	Inspector/Date	
<input type="checkbox"/>	Preliminary Notification/Report		Daily Report
<input checked="" type="checkbox"/>	Information Entered in RI Log		Review at Next Inspection
<input type="checkbox"/>	Report Referred To:		

3. REPORT EVALUATION

<input checked="" type="checkbox"/>	Description of Event	<input checked="" type="checkbox"/>	Corrective Actions
<input checked="" type="checkbox"/>	Levels of RAM Involved	<input checked="" type="checkbox"/>	Calculations Adequate
<input checked="" type="checkbox"/>	Cause of Event	<input checked="" type="checkbox"/>	Additional Information Requested from Licensee

4. MANAGEMENT DIRECTIVE 8.3 EVALUATION

<input type="checkbox"/>	Release w/Exposure > Limits	<input type="checkbox"/>	Deliberate Misuse w/Exposure > Limits
<input type="checkbox"/>	Repeated Inadequate Control	<input type="checkbox"/>	Pkging Failure > 10 rads/hr or Contamination > 1000x Limits
<input type="checkbox"/>	Exposure 5x Limits	<input type="checkbox"/>	Large# Indivs w/Exp > Limits or Medical Deterministic Effects
<input type="checkbox"/>	Potential Fatality	<input type="checkbox"/>	Unique Circumstances or Safeguards Concerns
If any of the above are involved:			
<input type="checkbox"/>	Considered Need for IIT	<input type="checkbox"/>	Considered Need for AIT
Decision/Made By/Date:			

5. MANAGEMENT DIRECTIVE 8.10 EVALUATION (additional evaluation for medical events only)

<input type="checkbox"/>	Timeliness - Inspection Meets Requirements (5 days for overdose / 10 days for underdose)
<input type="checkbox"/>	Medical Consultant Used-Name of Consultant/Date of Report:
<input type="checkbox"/>	Medical Consultant Determined Event Directly Contributed to Fatality
<input type="checkbox"/>	Device Failure with Possible Adverse Generic Implications
<input type="checkbox"/>	HQ or Contractor Support Required to Evaluate Consequences

6. SPECIAL INSTRUCTIONS OR COMMENTS

Similar event reported from 9/21/16, also involving WFS at JFK airport
--

<input type="checkbox"/> Non-Public	Inspector Signature:	Date:	1/12/17
<input checked="" type="checkbox"/> Public-SUNSI REVIEW COMPLETE	Branch Chief Initials:	Date:	1/13/17
Location of File: G:\REFERENCE\BLANK FORMS\MLER FORM.DOC			Rev. 09/12/13



Agilent Technologies

2850 Centerville Road
Wilmington, DE 19808

REC RG 1 01 06 17 PM 03:14

January 5, 2017

USNRC, Region I,
2100 Renaissance Boulevard, Suite 100
King of Prussia, PA 19406-2713

Subject: Notification of loss of licensed material

To Whom It May Concern,

In accordance with 10 CFR 20.2201, Agilent Technologies, Inc. (Agilent), wishes to report the loss of two Electron Capture Detectors (ECDs), each containing a 15 millicurie Nickel 63 (Ni-63) source.

Agilent manufactures ECDs in its Shanghai, China facility and ships completed product around the world. A small number of ECDs are shipped to the Agilent Little Falls site in Wilmington, DE for installation in gas chromatograph instruments which are typically sold only to U.S. customers. The standard practice is that the ECDs are transported in bulk by air from China to JFK International Airport and turned over to a warehouse at JFK managed by Worldwide Flight Services (WFS). The ECDs are delivered to the Little Falls site by UPS or FedEx traceable mail. In this case, there apparently was a deviation in the handoff between the airline and WFS warehouse as the two ECDs were not received by the warehouse. This is the same warehouse that lost an ECD on September 21st of 2016 (reference notification letter dated November 18, 2016).

Please accept the answers provided below to the questions listed in 10 CFR 20.2201.

(i) A description of the licensed material involved, including kind, quantity, and chemical and physical form:

Answer:

Each ECD contains a solid source plated with 15 millicuries of Nickel 63 (Ni-63).

(ii) A description of the circumstances under which the loss or theft occurred:

Answer: The shipment contained 2 boxes with one ECD in each box. The Shanghai airport provided video confirmation that the two ECDs were loaded onto the aircraft, so the current assumption is that the ECDs were lost sometime after arriving at JFK and being checked in by WFS.

(iii) A statement of disposition, or probable disposition, of the licensed material involved:

Answer:

Agilent's freight logistics service provider (Kintetsu World Express) has petitioned Worldwide Flight Services for this answer but has not received one to date.

(iv) Exposures of individuals to radiation, circumstances under which the exposures occurred, and the possible total effective dose equivalent to persons in unrestricted areas:

Answer:

There have been no known occurrences of exposure to individuals. The ECD is considered a sealed source. The Ni-63 source is embedded within a stainless steel cylinder that is kept closed by 4 tamper resistant screws. More information on the ECD and its characteristics may be found in the enclosed NRC REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES NR-0348-D-111-B. Please refer to the SAFETY ANALYSIS SURVEY (page 8 of 11) for a full description of possible exposure amounts to persons in unrestricted areas.

(v) Actions that have been taken, or will be taken, to recover the material:

Answer:

Agilent has received notice that multiple searches have been made at the Worldwide Flight Services warehouse. Additionally, as one of the ECDs identified in the letter dated November 18th, 2016 referenced on page 1 was miss-directed to the United States Postal Service (USPS), separate searches of the USPS warehouse were performed to locate the two missing ECDs, with no success.

(vi) Procedures or measures that have been, or will be, adopted to ensure against a recurrence of the loss or theft of licensed material:


Answer:

- Agilent has committed to, and is in final stages of, terminating services by Worldwide Flight Services at JFK and transferring inbound handling to a different company's warehouse at O'Hare International Airport in Chicago IL. Agilent will follow this written notice with confirmation of the change when it has been put into place.

- The air transporter used by Agilent to transport from Shanghai to the U.S. has made changes in their operational handling SOP's to improve communication and recovery to prevent future loss incidents

Please let me know if you have any questions.

Sincerely yours,

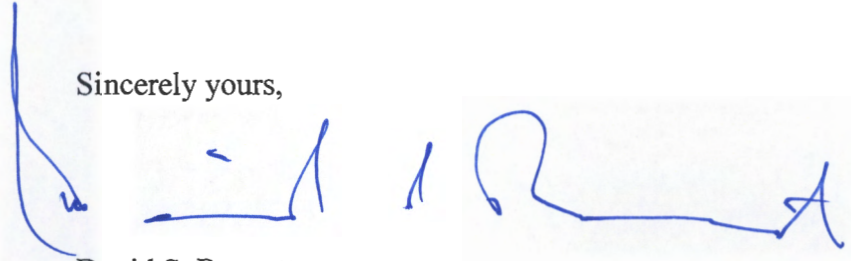A handwritten signature in blue ink, appearing to read 'David S. Bennett', is written over a light blue rectangular background.

David S. Bennett
Radiation Safety Officer
302-636-8262
david_bennett@agilent.com

C.c. David Hoppy
EHS Manager, Eastern Region

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 1 of 11

DEVICE TYPE: Electron Capture Detector

MODELS: G1223A, G1533A, G2310A, G2330A, G2397A, G2398A, G2404A,
G2405A, **G4597A, G4598A** (Generally Licensed)

G1224A, G1536A (Specifically Licensed)

DISTRIBUTOR:

Agilent Technologies, Inc.
Little Falls Site (previously Hewlett-
Packard, Little Falls Site)
2850 Centerville Road
Wilmington, DE 19808

MANUFACTURER:

Agilent Technologies, Shanghai Company
Limited
412 Ying Lun Road
Pu Dong
Shanghai, China

SEALED SOURCE MODEL
DESIGNATION:

QSA Global (formerly AEA
Technology) Model: NBCD

Eckert & Ziegler Isotope Products
(formerly Isotope Products
Laboratories) Model: NER-004P

ISOTOPE:

MAXIMUM ACTIVITY:

Nickel-63

18 mCi (0.67 GBq), Models G1223A, G1533A,
G1224A, G1536A

Nickel-63

15 mCi (0.56 GBq), Models G2397A, G2398A,
G2404A, G2405A, **G4597A, G4598A**

Nickel-63

5 mCi (185 MBq), Models G2301A, G2330A

LEAK TEST FREQUENCY:

6 months

PRINCIPAL USE:

(N) Ion Generator, Chromatography

CUSTOM DEVICE:

 YES X NO

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 2 of 11

DEVICE TYPE: Electron Capture Detector

DESCRIPTION:

The electron capture detectors (ECD's) that are registered in this certificate are devices that utilize sources manufactured by vendors listed on Page 1. The sources are registered separately and were found suitable for use in applications for chromatography ion generators.

The Models G1223A and G1224A electron capture detector (ECD) assemblies are similar to the previously approved Models 19233 and 19235. The model G1223A will be distributed to persons generally licensed and the Model G1224A will be distributed to persons specifically licensed. The two detectors are the same except that the detector label plate is different for general licenses versus specific licenses. The Models G1223A and G1224A ECDs are for use on the Model 5890 Series gas chromatographs. The manufacture of Model G1223A has been discontinued as of March 1, 2004.

The specific differences of the Models G1223A and G1224A relative to the Models 19223 and 19235 are as follows:

1. The detector heat sink is made of aluminum rather than stainless steel. The new heat sink allows the distributor to down rate their heater from 70 watts to 60 watts. This also limits the maximum temperature of the detector. In the event of a catastrophic failure mode, the 5890 gas chromatograph instrument's main processor would detect a shorted sensor fault, and turn off all heaters to devices on the gas chromatograph.
2. A 17-4 PH stainless steel will be used rather than 303 stainless steel. The supplier of the lower plated block, Amersham Corporation, has indicated that the plating quality of Ni-63 is better with 17-4 PH stainless steel. A 17-4 PH stainless steel lower block is currently being used on Models 19303 and 19312 ECD's. The inside of the lower block will be plated with non-radioactive nickel prior to plating of the Ni-63 radionuclide.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 3 of 11

DEVICE TYPE: Electron Capture Detector

DESCRIPTION (Cont.):

3. A metal seal will be used between the lower block (cathode) and the upper block (anode) that is currently used on other ECDs being distributed (for example, Models 18713A, 19282 and 18803-60520). This particular seal uses a silver crushable O-ring. The same tamper proof screws now used on all of the distributor's distributed ECDs will be used.
4. The upper anode block design has been redesigned. The non-plated part has reduced mass, a purged anode which has been raised (withdrawn) from the region of the Ni-63 plating within the lower block (cathode). The purged anode remains cleaner and is retained with a special nut and seal removable only with the distributor's anode wrench.
5. The outer cover and insulation are different than the 19233 and 19235 merely to accommodate the new gas chromatograph. The detector label plates will have the same information as our current detectors and will remain permanently attached to a tamper proof screw.

The Models G1533A and G1536A ECD assemblies are same as the Models G1223A and G1224A with the exception of modifications to the mounting hardware and the outer cover and insulation for use with a different gas chromatograph. The Model G1533A will be distributed to persons generally licensed and the Model G1536A will be distributed to persons specifically licensed. The two detectors are the same except that the detector label plate is different for general licenses versus specific licenses. The Models G1533A and G1536A ECDs are for use on the distributor's Model 6890 gas chromatographs.

The Models G2310A and G2330A are identical to the Models G1533A and G1223A respectively, except that the G2310A and G2330A will only contain up to 5 mCi (185 MBq) of Ni-63. The sources will be plated in the same manner as those in the Models G1533A and G1223A.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 4 of 11

DEVICE TYPE: Electron Capture Detector

DESCRIPTION (Cont.):

Models G2397A, G2398A, G2404A, and G2405A are almost identical to the ECD's described above. These ECDs still contain up to 15 mCi (555 MBq) of Ni-63, but instead of being plated onto the lower cell body the radioactive material is plated on a thin nickel cylinder. The cylinder is then press-fitted into the stainless steel lower body. The Model G2397A ECD is for use on the distributor's Models 6850, 6890, and 7890 gas chromatographs. The Model G2398A is for use on the distributor's Model 6890 gas chromatograph.

The upper body then attaches to the lower body with the same tamper-proof screws used in all designs. All ten ECDs are approximately 4" (10 cm) long and 1-1/8" (2.86 cm) in diameter at their widest location. General licensees never receive the tamper proof screws wrench or solvent cleaning/disassembly instructions.

Prior to 2000, the devices were distributed under the company name "Hewlett Packard". In 2000, the company split and the products were manufactured under the new company name of "Agilent Technologies". Agilent Technologies accepts returns of both Hewlett Packard and Agilent Technologies devices. The devices are cleaned and refurbished, then redistributed as initial distributions to new recipients.

Models G4597A and G4598A share the same internal ECD cell and tamper-resistant designs as Models G2397A, G2398A, G2404A, and G2405A. The ECD cell consists of a lower body that contains the Ni-63 capped with the upper body and sealed with an O-ring and tamper resistant screws. The ECD bottom aluminum block assembly contains a 60W Cartridge Heater/Sensor. The ECD top aluminum block contains the heater sensor, it also contains the relief bracket that protects the gas tubing, and covers the ECD cell. The ECD bottom and top blocks are fastened together with tamper-resistant screws. The main difference from the other models is that both Models G4597A and G4598A supply a path for make-up gas which is integrated into the ECD upper and lower body parts.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 5 of 11

DEVICE TYPE: Electron Capture Detector

DESCRIPTION (Cont.):

Models G4597A and G4598A utilize source Model NER-004P with a maximum activity of 15 mCi of Ni-63. Agilent Technologies reported that the only difference between the Models G4597A and G4598A is the model number, which is due to marketing purposes. Models G4597A and G4598A will be distributed to persons generally licensed and is for use in the Model 9000 Gas Chromatograph System.

LABELING:

Each **ECD** is stamped with the radiation symbol, the words, "Caution-Radioactive Material," the isotope and activity. Label plates are attached by cable to a tamper proof screw on the detector body. Users are instructed not to remove these plates. The plate contains the radiation symbol, the words, "Caution-Radioactive Material," the isotope, activity, model number, serial number, date, the words, "Electron Capture Detector," and the distributor name and logo. Additionally, for the Models used by general licensees, the plate contains the labeling requirements of 10 CFR 32.51(a), and refers the user to an instruction manual that tells them not to open or chemically clean the cell.

Devices distributed as of 2000 list "Agilent Technologies". Prior to 2000, the devices were distributed under the company name "Hewlett Packard", and the distributor is listed as "Hewlett Packard". Detector cells that had initially been distributed by "Hewlett Packard", and that are redistributed by "Agilent Technologies", list the distributor as "Agilent Technologies (Original Manufacturer: Hewlett-Packard Co.)", and indicate the original Hewlett Packard serial number and manufacturing date, in order to maintain traceability and to preserve accurate age information.

DIAGRAM:

See Attachments 1-5.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 6 of 11

DEVICE TYPE: Electron Capture Detector

CONDITIONS OF NORMAL USE (Cont.):

Each ECD is designed to be used in conjunction with gas chromatographs in analytical laboratories. Each ECD will be used in laboratory environment and by persons trained in the use of gas chromatography equipment. The ECD will normally be operated at temperatures up to 410°C (770°F). The working life of **all ECD Models** is 10 years.

PROTOTYPE TESTING:

Hewlett Packard tested the detector cells G1223A, G1533A, G2330A, G2310A, G1224A and G1536A to the criteria used on their presently licensed detector cells. The tests consisted of:

- Pressure test to 60 psi (414 kPa).
- Drop test from 1.5 meters (59").
- Vibration test to 55 Hz with an amplitude of 0.015" (0.38 mm).
- Freeze test to -40°C (-40°F).
- Loss of Ni-63 in carrier gas during normal use.
- Loss of Ni-63 from detector when all heat control systems fail.
- Loss of Ni-63 during solvent cleaning of the detector.
- Loss of Ni-63 at abnormally high temperatures (625°C [1157°F] and 800°C [1472°F]).

The sealed sources used in the ECD's meet the above tests and exceed the minimum ISO 2919 classification of C32211 for ion generators chromatography.

The following tests were performed on the G2397A, G2398A, G2404A, and G2405A designs: drop, impact, pressure, elevated temperature, and freeze. Because the ECDs are similar to the approved designs, no further testing was deemed necessary.

The manufacturer reported that the ECD cell for Models G4597A and G4598A have been tested to ISO 2919:2012 and achieved a classification of C42211.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 7 of 11

DEVICE TYPE: Electron Capture Detector

EXTERNAL RADIATION LEVELS:

The distributor has reported that radiation levels on all accessible surfaces do not exceed background levels for measurements taken from a detector with 18 mCi (666 MBq) of Ni-63. Attachment 3 is a dose rate report showing dose rate from an opened detector cell.

QUALITY ASSURANCE AND CONTROL:

The distributor maintains an ISO 9001 quality assurance and control program which has been deemed acceptable for licensing purposes by NRC.

LIMITATIONS AND/OR OTHER CONSIDERATIONS OF USE:

- The Models G1224A and G1536A shall be distributed only to persons specifically licensed by the NRC or an Agreement State.
- The Models G1223A, G1533A, G2310A, G2330A, G2397A, G2398A, G2404A, and G2405A shall be distributed to persons generally licensed by the NRC or an Agreement State.
- Handling, storage, use, transfer, and disposal: To be determined by the licensing authority or as required by 10 CFR 31.5 or Agreement State equivalent.
- The devices shall be leak tested at intervals not to exceed 6 months using techniques capable of detecting 0.005 mCi (185 Bq) of removable contamination.
- The user may install the device into gas chromatographs. However, the device may not be dismantled in any way by the user unless he obtains a specific license from NRC or an Agreement State to perform such activities.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 8 of 11

DEVICE TYPE: Electron Capture Detector

LIMITATIONS AND/OR OTHER CONSIDERATIONS OF USE (Cont.):

- This registration sheet and the information contained within the references shall not be changed without the written consent of the NRC.
- Reviewer's Note: The use of Model NBCD source, manufactured by QSA Global, Inc., was discontinued in June 2009, by Agilent Technologies, Inc. **ECDs Models containing the Model NBCD source are no longer commercially distributed but may be approved for licensing purposes.**
- Reviewer's Note: Agilent Technologies would audit the plated source supplier every two years starting from the last audit report dated February 12, 2009.
- Reviewer's Note: In letter dated January 15, 2015, Agilent informed the NRC that the ECD Models G2404A and G2405A were never introduced to the market and that no longer plans to manufacture or commercially distribute these products.

SAFETY ANALYSIS SUMMARY:

The distributor has submitted sufficient information to provide reasonable assurance that:

- The device can be safely operated by persons not having training in radiological protection.
- Under ordinary conditions of handling, storage, and use of the device, the byproduct material contained in the device will not be released or inadvertently removed from the source housing, and it is unlikely that any person will receive in any period of one year a dose in excess of 10 percent of the limits specified in Section 20.1201(a), 10 CFR Part 20.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 9 of 11

DEVICE TYPE: Electron Capture Detector

SAFETY ANALYSIS SUMMARY (Cont.):

- Under accident conditions associated with handling, storage, and use of the source housing, it is unlikely that any person would receive an external radiation dose or dose commitment in excess of the dose to the appropriate organ as specified in the following Table:

Table 1: External Radiation Dose

PART OF BODY	DOSE
Whole body; head and trunk active blood-forming organs gonads; or lens of eye	15 rem (0.15 Sv)
Hands and forearms; feet and ankles; localized areas of skin averaged over areas no larger than 1 square centimeter	200 rem (2.0 Sv)
Other Organs	50 rem (0.50 Sv)

Based on review of the ECD Models listed in this certificate of registration, and the information and test data cited below, we continue to conclude that the devices are acceptable for licensing purposes.

Furthermore, we continue to conclude that the devices would be expected to maintain their containment integrity for normal conditions of use and accidental conditions which might occur during uses specified in this certificate.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 10 of 11

DEVICE TYPE: Electron Capture Detector

REFERENCES:

The following supporting documents for the ECDs are hereby incorporated by reference and are made a part of this registry document.

- Hewlett-Packard's letters dated January 30, 1990, February 2, 1990, May 9, 1990, September 17, 1990, October 3, 1990, October 10, 1990, June 8, 1994, August 4, 1995, April 9, 1996, May 6, 1996, June 19, 1996, August 19, 1999, and November 1, 1999, with enclosures thereto.
- Agilent Technologies' letters dated, February 21, 2002, October 24, 2001, October 19, 2001, September 4, 2001, March 9, 2001, March 5, 2001, May 24, 2000, March 2, 2000, February 18, 2000, November 21, 1999, November 15, 1999, and November 1, 1999, with enclosures thereto.
- Agilent Technologies' letter dated September 26, 2003, email dated February 27, 2004, and email dated March 31, 2004, with enclosures thereto.
- Agilent Technologies' letter dated November 6, 2006.
- Agilent Technologies' letter dated June 7, 2007, with enclosures thereto.
- Agilent Technologies' emails dated June 20, 2007, with enclosures thereto.
- Agilent Technologies' letter dated January 8, 2008, with enclosures thereto.
- Agilent Technologies' letter dated January 23, 2009, and June 1, 2009, with enclosures thereto.

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

PAGE 11 of 11

DEVICE TYPE: Electron Capture Detector

REFERENCES (Cont.):

- Agilent Technologies' letter dated October 14, 2009, and January 22, 2010, and enclosures thereto.
- Agilent Technologies' letter dated September 13, 2013, and February 6, 2014, with enclosures thereto.
- Agilent Technologies' email dated March 27, 2014, with enclosures thereto.
- **Agilent Technologies' letters dated January 15, 2015 (ML15021A122), and March 19, 2015 (ML15084A128), with enclosures thereto. Agilent Technologies' letters dated April 28, 2015 (ML15118A879), and May 13, 2015 (ML15133A329).**

ISSUING AGENCY:

U.S. Nuclear Regulatory Commission

Date: May 14, 2015

Reviewer: /RA/
Maria Arribas-Colon

Date: May 14, 2015


Concurrence: /RA/
Tomas Herrera

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

ATTACHMENT 1 of 5




Models G1223A, G1533A, G2310A, G2330A, G1224A, and G1536A

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

ATTACHMENT 2 of 5



Models G2397A, G2398A, G2404A, and G2405A

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

ATTACHMENT 3 of 5

NER-0348-W-02 RING SOURCE DOSE RATE REPORT



NOTES

Source: NIA-14 (1000) installed in the lower cell block

Beta dose rate measurements are performed with a standard
Type 1 film badge having 1 milligram/square centimeter filter.
Minimum detectable dose rate is 0.3 mR/hr.

Gamma dose rate measurements are performed with a standard
Type 1 film badge having 100 milligram/square centimeter filter.
Minimum detectable dose rate is 0.1 mR/hr.


Models G2397A, G2398A, G2404A, G2405A

REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)

NO.: NR-0348-D-111-B

DATE: May 14, 2015

ATTACHMENT 4 of 5





Model G4597A, G4598A



REGISTRY OF RADIOACTIVE SEALED SOURCES AND DEVICES
SAFETY EVALUATION OF A DEVICE
(AMENDED IN ITS ENTIRETY)
(CORRECTED PAGE ATTACHMENT 5 - JUNE 4, 2015)



NO.: NR-0348-D-111-B

DATE: May 14, 2015

ATTACHMENT 5 of 5

 CAUTION RADIOACTIVE MATERIAL 555 MEGABECQUERELS/ 15 MILLICURIES OF NICKEL-63 G2397A ELECTRON CAPTURE DETECTOR	
SERIAL NO.	DATE
 Agilent Technologies	
<p>⚠ SEE THE GC AND ECD MANUALS BEFORE OPERATING OR SERVICING THIS DEVICE</p> <p>THIS DEVICE MUST BE WIPE (RADIOACTIVE LEAK) TESTED AT INTERVALS NOT GREATER THAN SIX MONTHS</p> <p>THE RECEIPT, POSSESSION, USE AND TRANSFER OF THIS DEVICE ARE SUBJECT TO A GENERAL LICENSE OR THE EQUIVALENT, AND THE REGULATIONS OF THE U.S. NRC OR OF A STATE WITH WHICH THE NRC HAS ENTERED INTO AN AGREEMENT FOR THE EXERCISE OF REGULATORY AUTHORITY. OUTSIDE U.S. CONSULT THE APPROPRIATE AGENCIES TO DETERMINE THE EQUIVALENT REGULATIONS.</p> <p>THE LABEL SHALL BE MAINTAINED ON THIS DEVICE IN A LEGIBLE CONDITION. REMOVAL OF THIS LABEL IS PROHIBITED</p> <p style="text-align: right; font-size: small;">MADE IN CHINA</p>	

 CAUTION RADIOACTIVE MATERIAL 555 MEGABECQUERELS/ 15 MILLICURIES OF NICKEL-63 G2398A ELECTRON CAPTURE DETECTOR	
SERIAL NO.	DATE
 Agilent Technologies	
<p>⚠ SEE THE GC AND ECD MANUALS BEFORE OPERATING OR SERVICING THIS DEVICE</p> <p>THIS DEVICE MUST BE WIPE (RADIOACTIVE LEAK) TESTED AT INTERVALS NOT GREATER THAN SIX MONTHS</p> <p>THE RECEIPT, POSSESSION, USE AND TRANSFER OF THIS DEVICE ARE SUBJECT TO A GENERAL LICENSE OR THE EQUIVALENT, AND THE REGULATIONS OF THE U.S. NRC OR OF A STATE WITH WHICH THE NRC HAS ENTERED INTO AN AGREEMENT FOR THE EXERCISE OF REGULATORY AUTHORITY. OUTSIDE U.S. CONSULT THE APPROPRIATE AGENCIES TO DETERMINE THE EQUIVALENT REGULATIONS.</p> <p>THE LABEL SHALL BE MAINTAINED ON THIS DEVICE IN A LEGIBLE CONDITION. REMOVAL OF THIS LABEL IS PROHIBITED</p> <p style="text-align: right; font-size: small;">MADE IN CHINA</p>	

 CAUTION RADIOACTIVE MATERIAL 555 MEGABECQUERELS/ 15 MILLICURIES OF NICKEL-63 G4557A ELECTRON CAPTURE DETECTOR	
SERIAL NO.	DATE
 Agilent Technologies	
<p>⚠ SEE THE GC AND ECD MANUALS BEFORE OPERATING OR SERVICING THIS DEVICE</p> <p>THIS DEVICE MUST BE WIPE (RADIOACTIVE LEAK) TESTED AT INTERVALS NOT GREATER THAN SIX MONTHS</p> <p>THE RECEIPT, POSSESSION, USE AND TRANSFER OF THIS DEVICE ARE SUBJECT TO A GENERAL LICENSE OR THE EQUIVALENT, AND THE REGULATIONS OF THE U.S. NRC OR OF A STATE WITH WHICH THE NRC HAS ENTERED INTO AN AGREEMENT FOR THE EXERCISE OF REGULATORY AUTHORITY. OUTSIDE U.S. CONSULT THE APPROPRIATE AGENCIES TO DETERMINE THE EQUIVALENT REGULATIONS.</p> <p>THE LABEL SHALL BE MAINTAINED ON THIS DEVICE IN A LEGIBLE CONDITION. REMOVAL OF THIS LABEL IS PROHIBITED</p> <p style="text-align: right; font-size: small;">MADE IN CHINA</p>	

 CAUTION RADIOACTIVE MATERIAL 555 MEGABECQUERELS/ 15 MILLICURIES OF NICKEL-63 G4558A ELECTRON CAPTURE DETECTOR	
SERIAL NO.	DATE
 Agilent Technologies	
<p>⚠ SEE THE GC AND ECD MANUALS BEFORE OPERATING OR SERVICING THIS DEVICE</p> <p>THIS DEVICE MUST BE WIPE (RADIOACTIVE LEAK) TESTED AT INTERVALS NOT GREATER THAN SIX MONTHS</p> <p>THE RECEIPT, POSSESSION, USE AND TRANSFER OF THIS DEVICE ARE SUBJECT TO A GENERAL LICENSE OR THE EQUIVALENT, AND THE REGULATIONS OF THE U.S. NRC OR OF A STATE WITH WHICH THE NRC HAS ENTERED INTO AN AGREEMENT FOR THE EXERCISE OF REGULATORY AUTHORITY. OUTSIDE U.S. CONSULT THE APPROPRIATE AGENCIES TO DETERMINE THE EQUIVALENT REGULATIONS.</p> <p>THE LABEL SHALL BE MAINTAINED ON THIS DEVICE IN A LEGIBLE CONDITION. REMOVAL OF THIS LABEL IS PROHIBITED</p> <p style="text-align: right; font-size: small;">MADE IN CHINA</p>	

Example of Labels

Non-Agreement State	Event Number: 52410
Rep Org: AGILENT TECHNOLOGIES Licensee: AGILENT TECHNOLOGIES Region: 1 City: WILMINGTON State: DE County: License #: 07-28762-01 Agreement: N Docket: NRC Notified By: DAVID BENNETT HQ OPS Officer: VINCE KLCO	Notification Date: 12/07/2016 Notification Time: 09:15 [ET] Event Date: 11/07/2016 Event Time: [EST] Last Update Date: 12/07/2016
Emergency Class: NON EMERGENCY 10 CFR Section: 20.2201(a)(1)(ii) - LOST/STOLEN LNM>10X	Person (Organization): ART BURRITT (R1DO) NMSS_EVENTS_NOTIFICA (EMAI)

This material event contains a "Less than Cat 3 " level of radioactive material.

Event Text

LOST SOURCES

Agilent Technologies is a manufacturer of a part containing an electron capture detector (ECD) that fits into a gas chromatograph. The ECD contains an embedded sealed source (Ni-63; 15 milliCuries) and is manufactured in Shanghai, China and is transferred into the United States through the JFK Airport Worldwide Flight Services Warehouse. When the licensee's Philadelphia truck shipping service attempted to retrieve the two ECD sources at the JFK warehouse, the sources were discovered missing. The warehouse was searched without success.

The ECD source serial numbers are U30355 and U30356. The model number is 62397AECD.

Agilent Technologies holds an NRC license and is located at 2850 Centerville Road, Wilmington, DE 19808.

THIS MATERIAL EVENT CONTAINS A "LESS THAN CAT 3" LEVEL OF RADIOACTIVE MATERIAL

Sources that are "Less than IAEA Category 3 sources," are either sources that are very unlikely to cause permanent injury to individuals or contain a very small amount of radioactive material that would not cause any permanent injury. Some of these sources, such as moisture density gauges or thickness gauges that are Category 4, the amount of unshielded radioactive material, if not safely managed or securely protected, could possibly - although it is unlikely - temporarily injure someone who handled it or were otherwise in contact with it, or who were close to it for a period of many weeks. For additional information go to http://www-pub.iaea.org/MTCDD/publications/PDF/Pub1227_web.pdf

Single Event Report

NMED Item Number: 160513

Narrative:

Last Updated: 12/15/2016

Agilent Technologies reported the loss of two electron capture detectors (ECDs; Agilent Technologies model G2397A, serial #U30355 and U30356) and each contained a 555 MBq (15 mCi) Ni-63 source. The ECDs were manufactured in Shanghai, China, and transferred to the United States through the JFK Airport Worldwide Flight Services Warehouse. When Agilent Technologies' Philadelphia truck shipping service attempted to retrieve the two ECDs at the JFK warehouse, they were not located. The warehouse was searched without success.

Event Date: 11/07/2016 Date Reported to Agreement State:

Discovery Date: 11/07/2016 Date Reported to NRC:

12/07/2016

Licensee/Reporting Party Information:

Regulated By:	NRC	Reciprocity:	NONE
License Number:	07-28762-01	Name:	AGILENT TECHNOLOGIES, INC.
NRC Docket Number:	03032792	City:	WILMINGTON
NRC Program Code:	03214	State:	DE
NRC Region:	1		

Site of Event:

Site Name: QUEENS State: NY

Additional Involved Party:

License Number:	NON-LICENSEE	Name:	JFK AIRPORT WORLDWIDE FLIGHT SERVICES WAREHOUSE
NRC Docket Number:	NA	City:	QUEENS
NRC Program Code:	NA	State:	NY
NRC Region:	1		

Other Information:

NRC Reportable Event:	Y	Abnormal Occurrence:	N
Agreement State Reportable Event:	N	Investigation:	N
Atomic Energy Act Material:	Y	Record Complete:	N
Consultant Hired:	N	Event Closed by Region/State:	N

Event Type:

LAS - LOST/ABANDONED/STOLEN

Event Cause:

LAS

Cause: MANAGEMENT DEFICIENCY

Event IAEA Aggregate Category:

LAS

IAEA Aggregate Category: NA

Corrective Actions Information:

Event Type: Number: Action:

LAS 1 NOT REPORTED

Source/Radioactive Material Information:

LAS

Source Number: 1

Source/Material: SEALED SOURCE ECD Radionuclide:

NI-63

Manufacturer: NR

Activity (Ci):

0.015

Model Number: NR

IAEA Category:

NA

Serial Number: NR

LAS

Source Number: 2

Source/Material: SEALED SOURCE ECD Radionuclide:

NI-63

Manufacturer: NR

Activity (Ci):

0.015

Model Number: NR

IAEA Category:

NA

Serial Number: NR

Leak Test Results (uCi):

Device/Associated Equipment Information:

LAS

Device Number: 1

Device/Equipment: ELECTRON CAPTURE DETECTOR

Model Number: G2397A

Manufacturer: AGILENT TECHNOLOGIES

Serial Number: U30355

LAS

Device Number: 2

Device/Equipment: ELECTRON CAPTURE DETECTOR

Model Number: G2397A

Manufacturer: AGILENT TECHNOLOGIES

Serial Number: U30356

Reporting Requirement Information:Event
Type: Requirement:

LAS 20.2201(a)(1)(ii) - Lost, stolen, or missing licensed material in a quantity greater than 10 times the Appendix C quantities.

Keywords:

Event Type: Keyword:

LAS MATERIAL LOST AND NOT FOUND

Reference Documents:

Reference Document Number: Entry Date: Retraction Date: Type of Report:

EN52410

12/15/2016

EVENT NOTIFICATION

12/7/16



Home > NRC Library> Document Collections> Reports Associated with Events > Event Notification Reports > 2016 > December 15

Event Notification Report for December 15, 2016

U.S. Nuclear Regulatory Commission
Operations Center

Event Reports For
12/14/2016 - 12/15/2016

**** EVENT NUMBERS ****

524105241152430524325243352434

Non-Agreement State

Rep Org: AGILENT TECHNOLOGIES

Licensee: AGILENT TECHNOLOGIES

Region: 1

City: WILMINGTON State: DE

County:

License #: 07-28762-01

Agreement: N

Docket:

NRC Notified By: DAVID BENNETT

HQ OPS Officer: VINCE KLCO

Emergency Class: NON EMERGENCY

10 CFR Section:

20.2201(a)(1)(ii) - LOST/STOLEN LNM>10XNMSS_EVENTS_NOTIFICA (EMAI)

Event Number: 52410

Notification Date: 12/07/2016

Notification Time: 09:15 [ET]

Event Date: 11/07/2016

Event Time: [EST]

Last Update Date: 12/07/2016

Person (Organization):

ART BURRITT (R1DO)

This material event contains a "Less than Cat 3 " level of radioactive material.

Event Text

LOST SOURCES

Agilent Technologies is a manufacturer of a part containing an electron capture detector (ECD) that fits into a gas chromatograph. The ECD contains an embedded sealed source (Ni-63; 15 milliCuries) and is manufactured in Shanghai, China and is transferred into the United States through the JFK Airport Worldwide Flight Services Warehouse. When the licensee's Philadelphia truck shipping service attempted to retrieve the two ECD sources at the JFK warehouse, the sources were discovered missing. The warehouse was searched without success.

The ECD source serial numbers are U30355 and U30356. The model number is 62397AECD.

Agilent Technologies holds an NRC license and is located at 2850 Centerville Road, Wilmington, DE 19808.

THIS MATERIAL EVENT CONTAINS A "LESS THAN CAT 3" LEVEL OF RADIOACTIVE MATERIAL

Sources that are "Less than IAEA Category 3 sources," are either sources that are very unlikely to cause permanent injury to individuals or contain a very small amount of radioactive material that would not cause any permanent injury. Some of these sources, such as moisture density gauges or thickness gauges that are Category 4, the amount of unshielded radioactive material, if not safely managed or securely protected, could possibly - although it is unlikely - temporarily injure someone who handled it or were otherwise in contact with it, or who were close to it for a period of many weeks. For additional information go to http://www-pub.iaea.org/MTCD/publications/PDF/Pub1227_web.pdf

TOP

Non-Agreement State

Rep Org: ACRUEN USA INSPECTIONS

Licensee: ACRUEN USA INSPECTIONS

Region: 4

City: ANCHORAGE State: AK

County:

License #: 50-32443-01

Agreement: N

Docket:

NRC Notified By: CHRIS DIXON

HQ OPS Officer: KARL DIEDERICH

Emergency Class: NON EMERGENCY

10 CFR Section:

20.2201(a)(1)(ii) - LOST/STOLEN LNM>10XANGELA MCINTOSH (NMSS)

Event Number: 52411

Notification Date: 12/07/2016

Notification Time: 11:27 [ET]

Event Date: 12/07/2016

Event Time: 06:30 [YST]

Last Update Date: 12/07/2016

Person (Organization):

VINCENT GADDY (R4DO)

ANGELA MCINTOSH (NMSS)

NMSS_EVENTS_NOTIFIC (EMAI)

CNSC (CANADA) (FAX)

This material event contains a "Category 2 " level of radioactive material.

Event Text

RADIOGRAPHY CAMERA LOST WHEN BARGE SANK IN BERING SEA

At approximately 1030 EST, a QSA 880 industrial radiography camera containing an Ir-192 source of approximately 26.3 Ci (source serial number - 32186G) was lost when the barge named Exito sank in the Bering Sea outside Dutch Harbor, Alaska. The ship was in transit and the camera was stored in a pelican case and not in use, with the source in the protected position. There were no unintended exposures to individuals. The licensee has notified the local area Coast Guard command.

Notified the following Federal Agencies: DHS SWO, FEMA Ops Center, USDA Ops Center, HHS Ops Center, DOE Ops Center, DHS NICC Watch Officer, EPA EOC. Notified the following Federal Agencies via email only: FDA EOC, Nuclear SSA, FEMA National Watch Center, and DNDO-JAC.

THIS MATERIAL EVENT CONTAINS A "CATEGORY 2" LEVEL OF RADIOACTIVE MATERIAL

Category 2 sources, if not safely managed or securely protected, could cause permanent injury to a person who handled them, or were otherwise in contact with them, for a short time (minutes to hours). It could possibly be fatal to be close to

Single Event Report

NMED Item Number: 160439

Narrative:

Last Updated: 10/31/2016

Agilent Technologies reported the loss of an electron capture detector (ECD) that contained a 555 MBq (15 mCi) Ni-63 fully encapsulated source. Four ECDs were shipped at the same time from Shanghai, China, to Agilent. The ECDs were shipped by air freight. Three of the ECDs arrived in the beginning of October 2016. One ECD has not arrived and a search is being performed.

Event Date: 09/21/2016 Date Reported to Agreement State: 10/21/2016
Discovery Date: 10/21/2016 Date Reported to NRC: 10/21/2016

Licensee/Reporting Party Information:

Regulated By: NRC Reciprocity: NONE
License Number: 07-28762-01 Name: AGILENT TECHNOLOGIES, INC.
NRC Docket Number: 03032792 City: WILMINGTON
NRC Program Code: 03214 State: DE
NRC Region: 1

Site of Event:

Site Name: SHANGHAI State: CH

Additional Involved Party:

License Number: NA Name: NA
NRC Docket Number: NA City: NA
NRC Program Code: NA State: NA
NRC Region: NA

Other Information:

NRC Reportable Event:	Y	Abnormal Occurrence:	N
Agreement State Reportable Event:	N	Investigation:	N
Atomic Energy Act Material:	Y	Record Complete:	N
Consultant Hired:	N	Event Closed by Region/State:	N

Event Type:

LAS - LOST/ABANDONED/STOLEN

Event Cause:

LAS

Cause: NOT REPORTED

Event IAEA Aggregate Category:

LAS

IAEA Aggregate Category: NA

Corrective Actions Information:

Event Type: Number: Action:

LAS 1 NOT REPORTED

Source/Radioactive Material Information:

LAS

Source Number: 1

Source/Material: SEALED SOURCE ECD Radionuclide: NI-63

Manufacturer: AGILENT TECHNOLOGIES Activity (Ci): 0.015

Model Number: NR IAEA Category: NA

Serial Number: NR

Device/Associated Equipment Information:

LAS

Device Number: 1

Device/Equipment: ELECTRON CAPTURE DETECTOR Model Number: NR

Manufacturer: AGILENT TECHNOLOGIES Serial Number: NR

Reporting Requirement Information:Event
Type: Requirement:

LAS 20.2201(a)(1)(ii) - Lost, stolen, or missing licensed material in a quantity greater than 10 times the Appendix C quantities.

Keywords:

Event Type: Keyword:

LAS MATERIAL LOST AND NOT FOUND

Reference Documents:

Reference Document Number: Entry Date: Retraction Date: Type of Report:

EN52312

10/31/2016
10/21/16

EVENT NOTIFICATION

THIS MATERIAL EVENT CONTAINS A "LESS THAN CAT 3" LEVEL OF RADIOACTIVE MATERIAL

Sources that are "Less than IAEA Category 3 sources," are either sources that are very unlikely to cause permanent injury to individuals or contain a very small amount of radioactive material that would not cause any permanent injury. Some of these sources, such as moisture density gauges or thickness gauges that are Category 4, the amount of unshielded radioactive material, if not safely managed or securely protected, could possibly - although it is unlikely - temporarily injure someone who handled it or were otherwise in contact with it, or who were close to it for a period of many weeks. For additional information go to http://www-pub.iaea.org/MTCD/publications/PDF/Pub1227_web.pdf



TOP

Non-Agreement State

Rep Org: AGILENT

Licensee: AGILENT

Region: 1

City: WILMINGTON State: DE

County:

License #: 07-28762-01

Agreement: N

Docket:

NRC Notified By: DAVID BENNETT

HQ OPS Officer: MARK ABRAMOVITZ

Emergency Class: NON EMERGENCY

10 CFR Section:

20.2201(a)(1)(ii) - LOST/STOLEN LNM>10XNMSS_EVENTS_NOTIFICA (EMAI)

Event Number: 52312

Notification Date: 10/21/2016

Notification Time: 08:28 [ET]

Event Date: 09/21/2016

Event Time: [EDT]

Last Update Date: 10/21/2016

Person (Organization):

CHRISTOPHER CAHILL (R1DO)

This material event contains a "Less than Cat 3 " level of radioactive material.

Event Text

LOST ELECTRON CAPTURE DEVICE

Four electron capture detectors (ECDs) were shipped at the same time from Shanghai to Wilmington, DE. The ECDs were shipped by air freight and three of the ECDs arrived at the beginning of October. The remaining ECD has not arrived and a search is ongoing.

Source: Ni-63, 15 mCi fully encapsulated

THIS MATERIAL EVENT CONTAINS A "LESS THAN CAT 3" LEVEL OF RADIOACTIVE MATERIAL

Sources that are "Less than IAEA Category 3 sources," are either sources that are very unlikely to cause permanent injury to individuals or contain a very small amount of radioactive material that would not cause any permanent injury. Some of these sources, such as moisture density gauges or thickness gauges that are Category 4, the amount of unshielded radioactive material, if not safely managed or securely protected, could possibly - although it is unlikely - temporarily injure someone who handled it or were otherwise in contact with it, or who were close to it for a period of many weeks. For additional information go to http://www-pub.iaea.org/MTCD/publications/PDF/Pub1227_web.pdf



TOP

Agreement State

Event Number: 52313



Home > NRC Library> Document Collections> Reports Associated with Events > Event Notification Reports > 2016 > October 31

Event Notification Report for October 31, 2016

U.S. Nuclear Regulatory Commission
Operations Center

Event Reports For
10/28/2016 - 10/31/2016

**** EVENT NUMBERS ****

5231152312523135231452327523295233152332

TOP

Agreement State	Event Number: 52311
Rep Org: NE DIV OF RADIOACTIVE MATERIALS	Notification Date: 10/20/2016
Licensee: THE NEBRASKA MEDICAL CENTER	Notification Time: 15:16 [ET]
Region: 4	Event Date: 10/13/2016
City: OMAHA State: NE	Event Time: [CDT]
County:	Last Update Date: 10/20/2016
License #: 01-88-01	
Agreement: Y	
Docket:	
NRC Notified By: BRYAN MILLER	
HQ OPS Officer: STEVE SANDIN	
Emergency Class: NON EMERGENCY	Person (Organization):
10 CFR Section:	JOHN KRAMER (R4DO)
AGREEMENT STATE	NMSS_EVENTS_NOTIFIC (EMAI)

This material event contains a "Less than Cat 3 " level of radioactive material.

Event Text

AGREEMENT STATE REPORT - DIAGNOSTIC RADIOACTIVE SOURCE MISSING

On the morning of 10/13/16, a patient received a diagnostic 0.297 mCi I-125 seed implant to characterize a breast lesion. That afternoon, the tissue and implanted seed were removed and sent to pathology for assessment. The bio-waste was received in pathology as a non-radioactive sample contrary to hospital procedures. A subsequent search of the pathology lab could not locate the missing source.

The State of Nebraska was notified of the incident on 10/19/16.