

**MATERIALS LICENSE**


Pursuant to the Atomic Energy Act of 1954, as amended, the Energy Reorganization Act of 1974 (Public Law 93-438), and Title 10, Code of Federal Regulations, Chapter I, Parts 30, 31, 32, 33, 34, 35, 36, 37, 39, 40, 70 and 71, and in reliance on statements and representations heretofore made by the licensee, a license is hereby issued authorizing the licensee to receive, acquire, possess, and transfer byproduct, source, and special nuclear material designated below; to use such material for the purpose(s) and at the place(s) designated below; to deliver or transfer such material to persons authorized to receive it in accordance with the regulations of the applicable Part(s). This license shall be deemed to contain the conditions specified in Section 183 of the Atomic Energy Act of 1954, as amended, and is subject to all applicable rules, regulations, and orders of the Nuclear Regulatory Commission now or hereafter in effect and to any conditions specified below.

<b>Licensee</b>  1. PharmaLogic Michigan, L.L.C.  2. 1501 Cass St. Traverse City, MI 49686		In accordance with letter dated September 25, 2017.	4. Expiration Date: February 29, 2020
		3. License number: 21-32190-01MD is amended in its entirety to read as follows:	5. Docket No.: 030-35125 Reference No.:
6. Byproduct, source, and/or special nuclear material  A. Any byproduct material between Atomic Numbers 3 and 83 with Exceptions  B. Molybdenum-99 C. Technetium-99m D. Xenon-133 E. Iodine-131	7. Chemical and/or physical form  A. Any except sealed source  B. Any except sealed source C. Any except sealed source D. Any except sealed source E. Any except sealed source	8. Maximum amount that licensee may possess at any one time under this license  A. 200 millicuries per radionuclide; 2 curies total  B. 100 curies total C. 100 curies total D. 1.5 curies total E. 2.5 curies total	9. Authorized use  A. For preparation, distribution and redistribution of radioactive drugs, including compounding of Iodine-131 and redistribution of unused molybdenum-99/technetium-99m generators to authorized recipients, in accordance with 10 CFR 32.72 and for non-medical use to authorized recipients.  B. Same as Item 9.A. C. Same as Item 9.A. D. Same as Item 9.A. E. Same as Item 9.A.

**MATERIALS LICENSE  
SUPPLEMENTARY SHEET**License Number  
21-32190-01MD

Amendment No. 20

Docket or Reference Number  
030-35125

6. Byproduct, source, and/or special nuclear material
- F. Any byproduct material permitted by 10 CFR 31.11
- G. Any byproduct material identified in 10 CFR 35.400
- H. Any byproduct material permitted by 10 CFR 35.500
7. Chemical and/or physical form
- F. Prepackaged Kits
- G. Sealed Sources
- H. Sealed Sources
8. Maximum amount that licensee may possess at any one time under this license
- F. 50 millicuries total
- G. 500 millicuries total
- H. 1.5 curies per source and 5.5 curies total
9. Authorized use
- F. For redistribution to specific licensees or to general licensees in accordance with 10 CFR 31.11, provided the packaging and labeling remain unchanged.
- G. For redistribution of sealed sources initially distributed by a manufacturer licensed pursuant to 10 CFR 32.74. For redistribution of sealed sources that have been registered either with NRC under 10 CFR 32.210 or with an Agreement State and have been distributed in accordance with an NRC or Agreement State specific license authorizing distribution to persons specifically authorized by an NRC or Agreement State license to receive, possess and use the authorized device and to authorized recipients for non-medical use.
- H. Same as Item 9.G.
- 

# **MATERIALS LICENSE SUPPLEMENTARY SHEET**

License Number  
21-32190-01MD

Amendment No. 20

Docket or Reference Number  
030-35125

- |   |                                  |  |   |
|---|----------------------------------|--|---|
| 6. Byproduct, source, and/or special nuclear material   | 7. Chemical and/or physical form | 8. Maximum amount that licensee may possess at any one time under this license | 9. Authorized use   |
| I. Any byproduct material authorized under 10 CFR 35.65 | I. Sealed Sources                | I. 150 millicuries total   | I. For use in calibration and checking of the licensee's own dose calibrator and checking of the licensee's own radiation detection instruments. For redistribution of sealed sources initially distributed by a manufacturer licensed pursuant to 10 CFR 32.74 and for non-medical use to authorized recipients. |
| J. Samarium-153   | J. Any except sealed source      | J. 750 millicuries total   | J. Same as Item 9.A.  |
| K. Uranium- depleted in Uranium-235                     | K. Metal                         | K. 600 kilograms total   | K. For shielding for molybdenum-99/technetium-99m generators.   |
| L. Yttrium-90   | L. Any except sealed source      | L. 500 millicuries total   | L. Same as Item 9.A.  |
| M. Fluorine-18  | M. Any                           | M. 1 curie total   | M. For preparation and distribution of radioactive drugs and radiochemicals for medical use in accordance with 10 CFR 32.72 and for non-medical use to authorized recipients.   |
| N. Gallium-67   | N. Any                           | N. 500 millicuries total   | N. Same as Item 9.M.  |
| O. Indium-111   | O. Any                           | O. 300 millicuries total   | O. Same as Item 9.M.  |
| P. Thallium-201   | P. Any                           | P. 1 curie total   | P. Same as Item 9.M.  |

CONDITIONS

**MATERIALS LICENSE  
SUPPLEMENTARY SHEET**License Number  
21-32190-01MD

Amendment No. 20

Docket or Reference Number  
030-35125

10. Licensed material may be used or stored at the licensee's facilities located at 1501 Cass Street, Traverse City, Michigan.
11. The Radiation Safety Officer (RSO) for this license is Dana L. Suttle, R.Ph.
12. Licensed material shall only be used by, or under the supervision of:
- A. A pharmacist working or designated as an authorized nuclear pharmacist in accordance with 10 CFR 32.72(b)(2)(i) or (4).
- B. Authorized Nuclear Pharmacists:
- | <u>Authorized Nuclear Pharmacist</u> | <u>Material and Use</u> |
|--------------------------------------|-------------------------|
| William Marc Chatoff, R.Ph., BCNP    | All                     |
| Tom Defranco, R.Ph.                  | All                     |
| Dana Suttle, R.Ph.                   | All                     |
| James M. Bichler, R.Ph.              | All                     |
| Shawn Lorrain, R.Ph.                 | All                     |
| Gerald Strugala, R.Ph., BCNP         | All                     |
| Glen Palmer, R.Ph., BCNP             | All                     |
| Selina Mirjavadi, R.Ph.              | All                     |
| William Espie Gillette, R.Ph.        | All                     |
| Joseph Lofaro, R.Ph.                 | All                     |
| Tamiko Ushio, R.Ph.                  | All                     |
| Matthew Witt Hinton, R.Ph.           | All                     |
| Garth Kistner, R.Ph.                 | All                     |
| Richard Sucece, R.Ph.                | All                     |
| Laurie Stallings, R.Ph.              | All                     |

**MATERIALS LICENSE  
SUPPLEMENTARY SHEET**License Number  
21-32190-01MD

Amendment No. 20

Docket or Reference Number  
030-35125Authorized Nuclear Pharmacist

Ruth Mary Wetzel, R.Ph.

Logan William Payne, R.Ph.

Bynum L. Kimmons, R.Ph.

Material and Use

All

All

All

13. A. Sealed sources shall be tested for leakage and/or contamination at intervals not to exceed the intervals specified in the certificate of registration issued by the U.S. Nuclear Regulatory Commission under 10 CFR 32.210 or by an Agreement State. In the absence of a registration certificate, sealed sources shall be tested for leakage and/or contamination at intervals not to exceed 6 months, or at such other intervals as specified.
- B. In the absence of a certificate from a transferor indicating that a leak test has been made within the intervals specified in the certificate of registration issued by the U.S. Nuclear Regulatory Commission under 10 CFR 32.210 or by an Agreement State, prior to the transfer, a sealed source received from another person shall not be put into use until tested and the test results received.
- C. Sealed sources need not be tested if they contain only hydrogen-3; or they contain only a radioactive gas; or the half-life of the isotope is 30 days or less; or they contain not more than 100 microcuries of beta- and/or gamma-emitting material or not more than 10 microcuries of alpha-emitting material.
- D. Sealed sources need not be tested if they are in storage and are not being used. However, when they are removed from storage for use or transferred to another person, and have not been tested within the required leak test interval, they shall be tested before use or transfer. No sealed source shall be stored for a period of more than 10 years without being tested for leakage and/or contamination.
- E. The leak test shall be capable of detecting the presence of 185 becquerels (0.005 microcuries) of radioactive material on the test sample. If the test reveals the presence of 185 becquerels (0.005 microcuries) or more of removable contamination, a report shall be filed with the U.S. Nuclear Regulatory Commission in accordance with 10 CFR 30.50(c)(2), and the source shall be removed immediately from service and decontaminated, repaired, or disposed of in accordance with Commission regulations.

**MATERIALS LICENSE  
SUPPLEMENTARY SHEET**License Number  
21-32190-01MD

Amendment No. 20


Docket or Reference Number  
030-35125

- F. Tests for leakage and/or contamination shall be performed by the licensee or other persons specifically licensed by the U.S. Nuclear Regulatory Commission or an Agreement State to perform such services. In addition, the licensee is authorized to collect leak test samples for analysis by persons specifically licensed by the Commission or an Agreement State to perform such services.
- G. Records of leak test results shall be kept in units of becquerels (microcuries) and shall be maintained for 3 years.
14. Sealed sources containing licensed material shall not be opened or sources removed from source holders by the licensee, except as specifically authorized.
15. The licensee shall conduct a physical inventory every 6 months, or at other intervals approved by the U.S. Nuclear Regulatory Commission, to account for all sealed sources and/or devices received and possessed under the license. Records of inventories shall be maintained for 3 years from the date of each inventory, and shall include the radionuclides, quantities, manufacturer's name and model numbers, and the date of the inventory.
16. The licensee is authorized to hold radioactive material with a physical half-life of less than or equal to 120 days for decay-in-storage before disposal in ordinary trash provided:
- A. Before disposal as ordinary trash, the waste shall be surveyed at the container surface with the appropriate survey instrument set on its most sensitive scale and with no interposed shielding to determine that its radioactivity cannot be distinguished from background. All radiation labels shall be removed or obliterated, except for radiation labels on materials that are within containers and that will be managed as biomedical waste after they have been released from the licensee.
- B. A record of each such disposal permitted under this license condition shall be retained for 3 years. The record must include the date of disposal, the date on which the byproduct material was placed in storage, the radionuclides disposed, the survey instrument used, the background dose rate, the dose rate measured at the surface of each waste container, and the name of the individual who performed the disposal.

**MATERIALS LICENSE  
SUPPLEMENTARY SHEET**License Number  
21-32190-01MDDocket or Reference Number  
030-35125

Amendment No. 20

17. The licensee is authorized to retrieve, receive and dispose of radioactive waste from its customers, limited to radiopharmacy-supplied syringes and vials and their contents.
18. Except for maintaining labeling as required by 10 CFR Part 20, or Part 71, the licensee shall obtain authorization from the U.S. Nuclear Regulatory Commission before making any changes in the sealed source, device, or source-device combination that would alter the description or specifications as indicated in the respective certificate of registration issued either by the U.S. Nuclear Regulatory Commission pursuant to 10 CFR 32.210 or by an Agreement State.
19. This license does not authorize distribution to persons exempt from licensing.

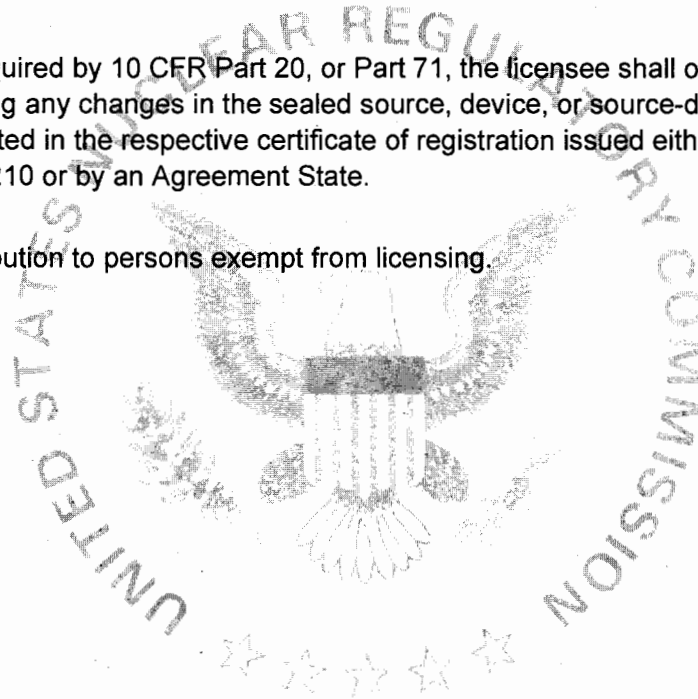


**MATERIALS LICENSE  
SUPPLEMENTARY SHEET**License Number  
21-32190-01MD

Amendment No. 20

Docket or Reference Number  
030-35125

20. Except as specifically provided otherwise in this license, the licensee shall conduct its program in accordance with the statements, representations, and procedures contained in the documents, including any enclosures, listed below. This license condition applies only to those procedures that are required to be submitted in accordance with the regulations. The U.S. Nuclear Regulatory Commission's regulations shall govern unless the statements, representations, and procedures in the licensee's application and correspondence are more restrictive than the regulations.

- A. Application dated January 19, 2010 (ML100340126)
- B. Letter dated June 22, 2012 (ML12177A413)
- C. Letter dated August 27, 2012 (ML12264A148)
- D. Letter dated August 30, 2012 (ML12264A142)
- E. Letter dated September 14, 2012 (ML12261A459)
- F. Facsimile dated February 16, 2010 (ML100480153)
- G. Letter dated September 25, 2017 (ML17270A377)



FOR THE U.S. NUCLEAR REGULATORY COMMISSION

Date: DEC 06 2017

By: \_\_\_\_\_

Bryan A. Parker  
Region 3