

**HARTFORD
MEMORIAL
HOSPITAL**
INCORPORATED

June 3, 1985

U. S. Nuclear Regulatory Commission
Radioisotopes Licensing Section
Region III
799 Roosevelt Road
Glen Ellyn, Illinois 60137

Re: Amendment to NRC Radioactive Materials License #48-18037-01

Gentlemen:


We request amendment to our Radioactive Materials License #48-18037-01 for the following:

CHANGE IN LOCATION OF NUCLEAR MEDICINE DEPARTMENT: Enclosed please find a facility sketch representing the design of our new Nuclear Medicine Department.

We confirm a "close-out radiation survey" of the current facilities will be performed before that area is released for unrestricted use. Records of this survey will be maintained at our hospital for NRC inspection. Action levels will be < 0.05 mr/hr as measured with a low level G.M. Survey meter and 200 DPM/100cm², as measured with a well counter. The NRC "Guide for Decontamination of Facilities" dated July 1982, will be followed.

We trust the information contained herein is sufficient to grant our request for this amendment. We look forward to receipt of that document.

Sincerely,



James E. Lyons
President

:amw

B507160007 B50613
REG3 LIC30
48-18037-01 PDR


RECEIVED
JUN 04 1985
REGION III

CONTROL NO. 79117

Hartford Memorial Hospital
Hartford, Wisconsin

SCALE
 $\frac{1}{4}" = 1'0"$

RECOVERY

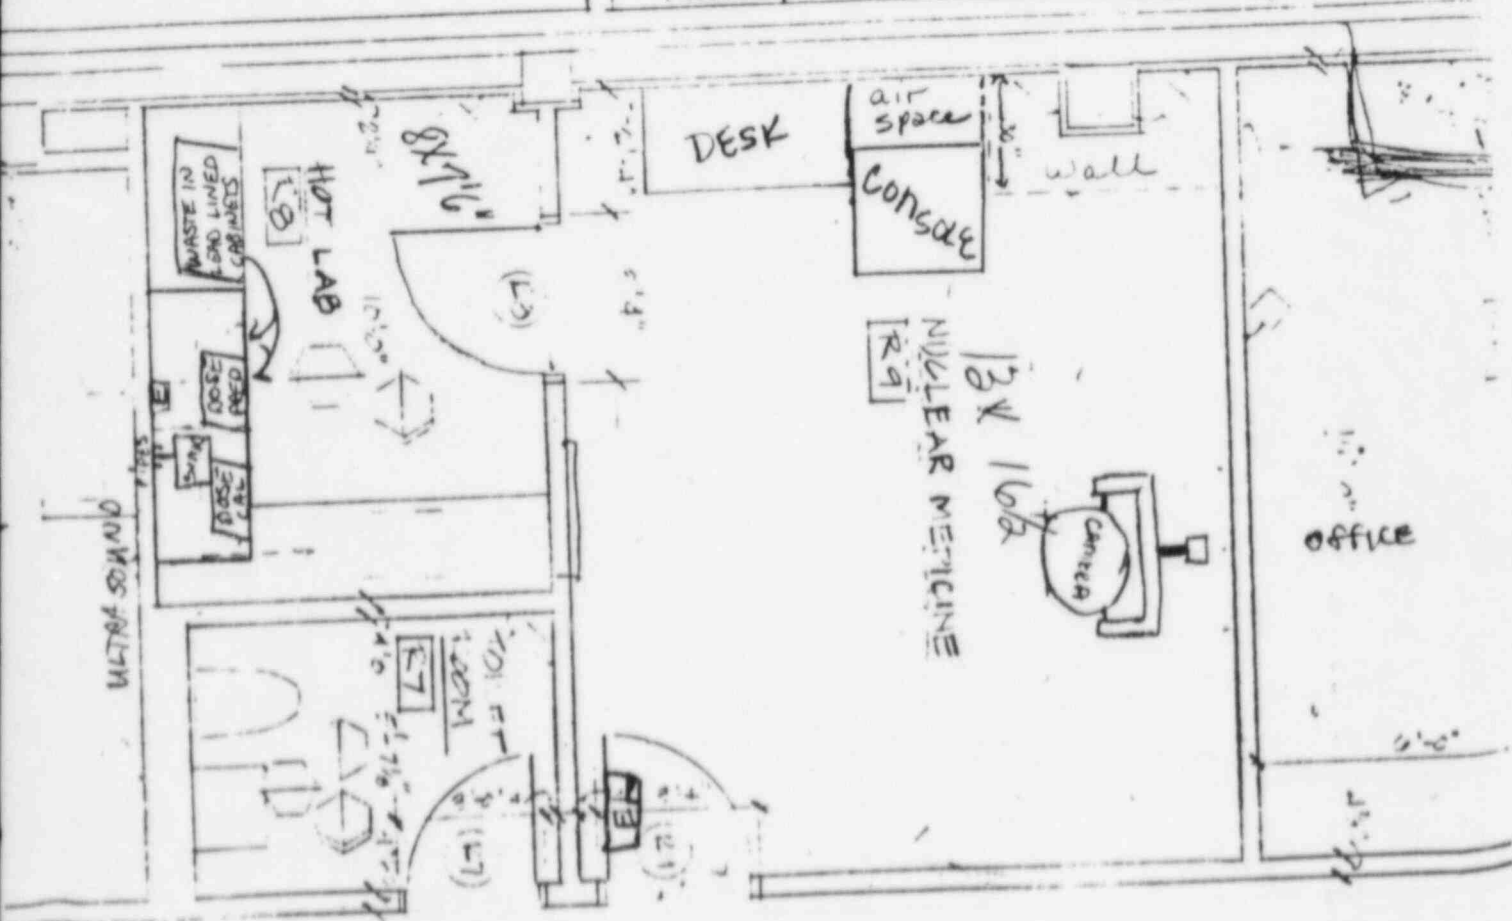

$8'4"$

CORRIDOR
DOOR
LOCK

CONTROL NO. 79117

**HARTFORD
MEMORIAL
HOSPITAL**
INCORPORATED

June 3, 1985

U. S. Nuclear Regulatory Commission
Radioisotopes Licensing Section
Region III
799 Roosevelt Road
Glen Ellyn, Illinois 60137

Applicant	<i>June 12th</i>
Check No.	<i>48249 \$120</i>
Amount	<i>72</i>
Type	<i>Amend</i>
Date Check Rec'd	<i>6/17/85</i>
Received By	<i>[Signature]</i>

Re: Amendment to NRC Radioactive Materials License #48-18037-01

Gentlemen:

We request amendment to our Radioactive Materials License #48-18037-01 for the following:

CHANGE IN LOCATION OF NUCLEAR MEDICINE DEPARTMENT: Enclosed please find a facility sketch representing the design of our new Nuclear Medicine Department.

We confirm a "close-out radiation survey" of the current facilities will be performed before that area is released for unrestricted use. Records of this survey will be maintained at our hospital for NRC inspection. Action levels will be <0.05 mr/hr as measured with a low level G.M. Survey meter and $200 \text{ DPM}/100\text{cm}^2$, as measured with a well counter. The NRC "Guide for Decontamination of Facilities" dated July 1982, will be followed.

We trust the information contained herein is sufficient to grant our request for this amendment. We look forward to receipt of that document.

Sincerely,

James E. Lyons
James E. Lyons
President

:amw

RECEIVED

JUN 04 1985

REGION III

RECEIVED


'85 JUN 17 P2:48

U.S. N.R.C.
LIC. FEE MGMT. BRANCH

CONTROL NO. 79117

JUN 4 1985

$\frac{1}{4}'' = 1'0''$
SCALE

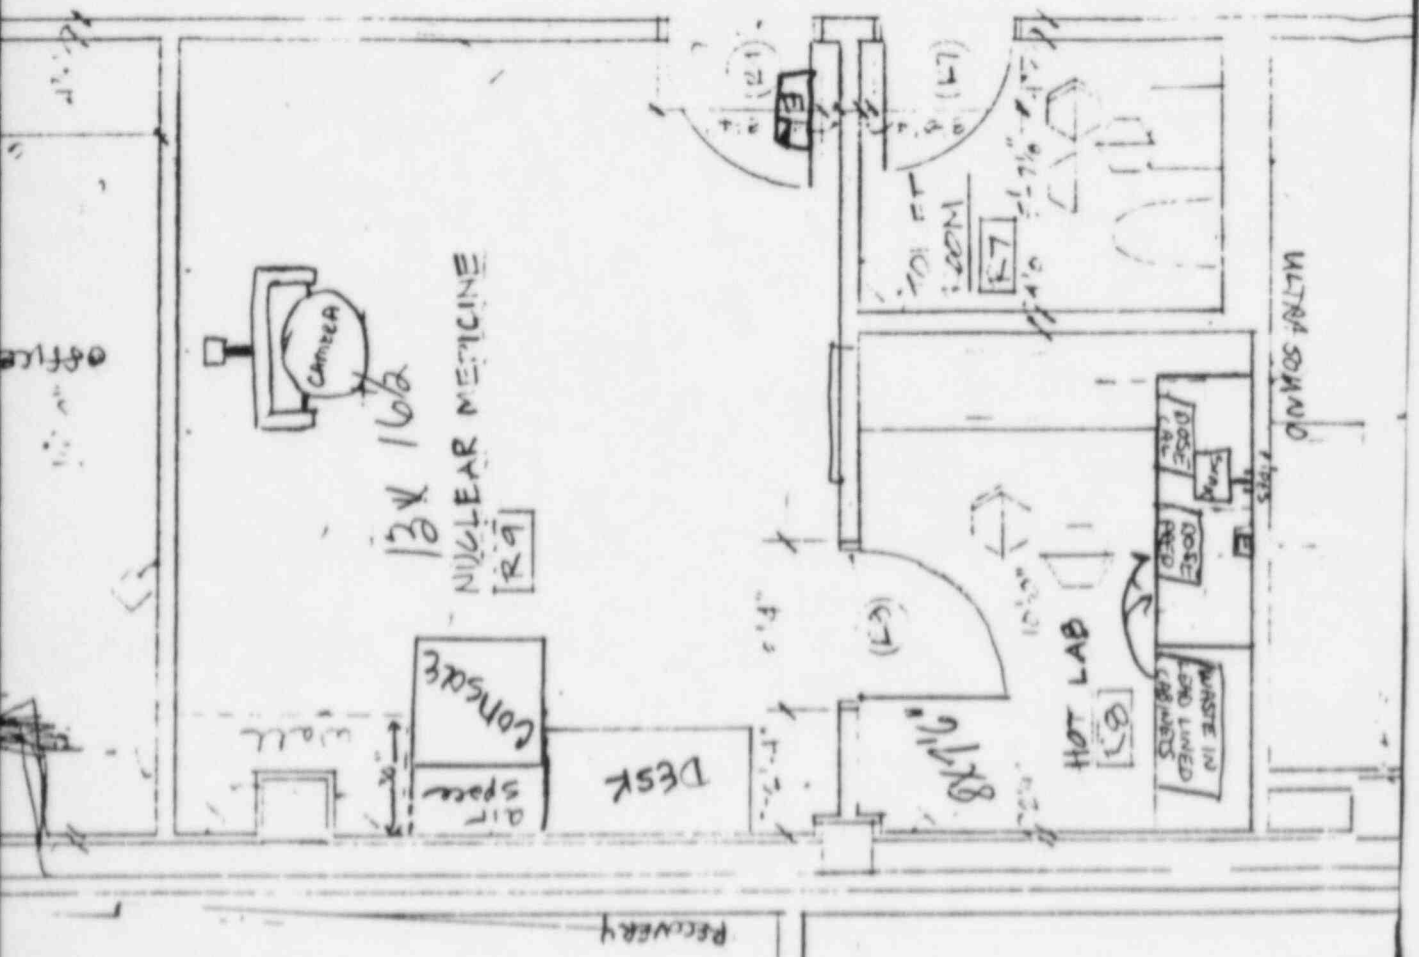

8 ft. →

CORR. DOOR

ULTRASOUND

HOT LAB

NUCLEAR MEDICINE

CAMERA

13x16

DESK

AIR SPACE

WALL

WASTE IN LEAD LINED CABINETS

DOSE RATE

RECOVERY

OFFICE