


ST. JOHN MEDICAL CENTER • 1923 SOUTH UTICA AVENUE • TULSA, OKLAHOMA 74104 • 918 / 744-2345

June 6, 1985

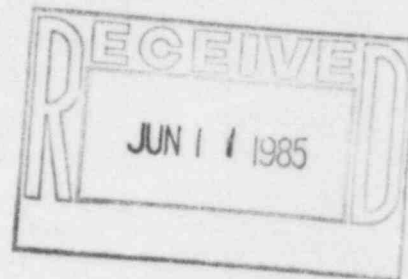

Mr. Jack Whitten  
U.S. Nuclear Regulatory Commission  
611 Ryan Plaza Drive, Suite 1000  
Arlington, Texas 76016

RE: License #35- 00376-05

Dear Mr. Whitten:

Attached are the floor diagrams that were inadvertently not included in our letter to you of April 26, 1985 concerning the installation of a new Cobalt-60 Source.

We wish to correct the source model number listed in item H of our previous letter. The source model number is NPI-20-7000W.

Sincerely,


*Keith M. Jones, PhD*

Keith M. Jones, Ph.D.  
Radiation Physicist

8508280205 850715  
REG4 LIC30  
35-00376-05 PDR



460619

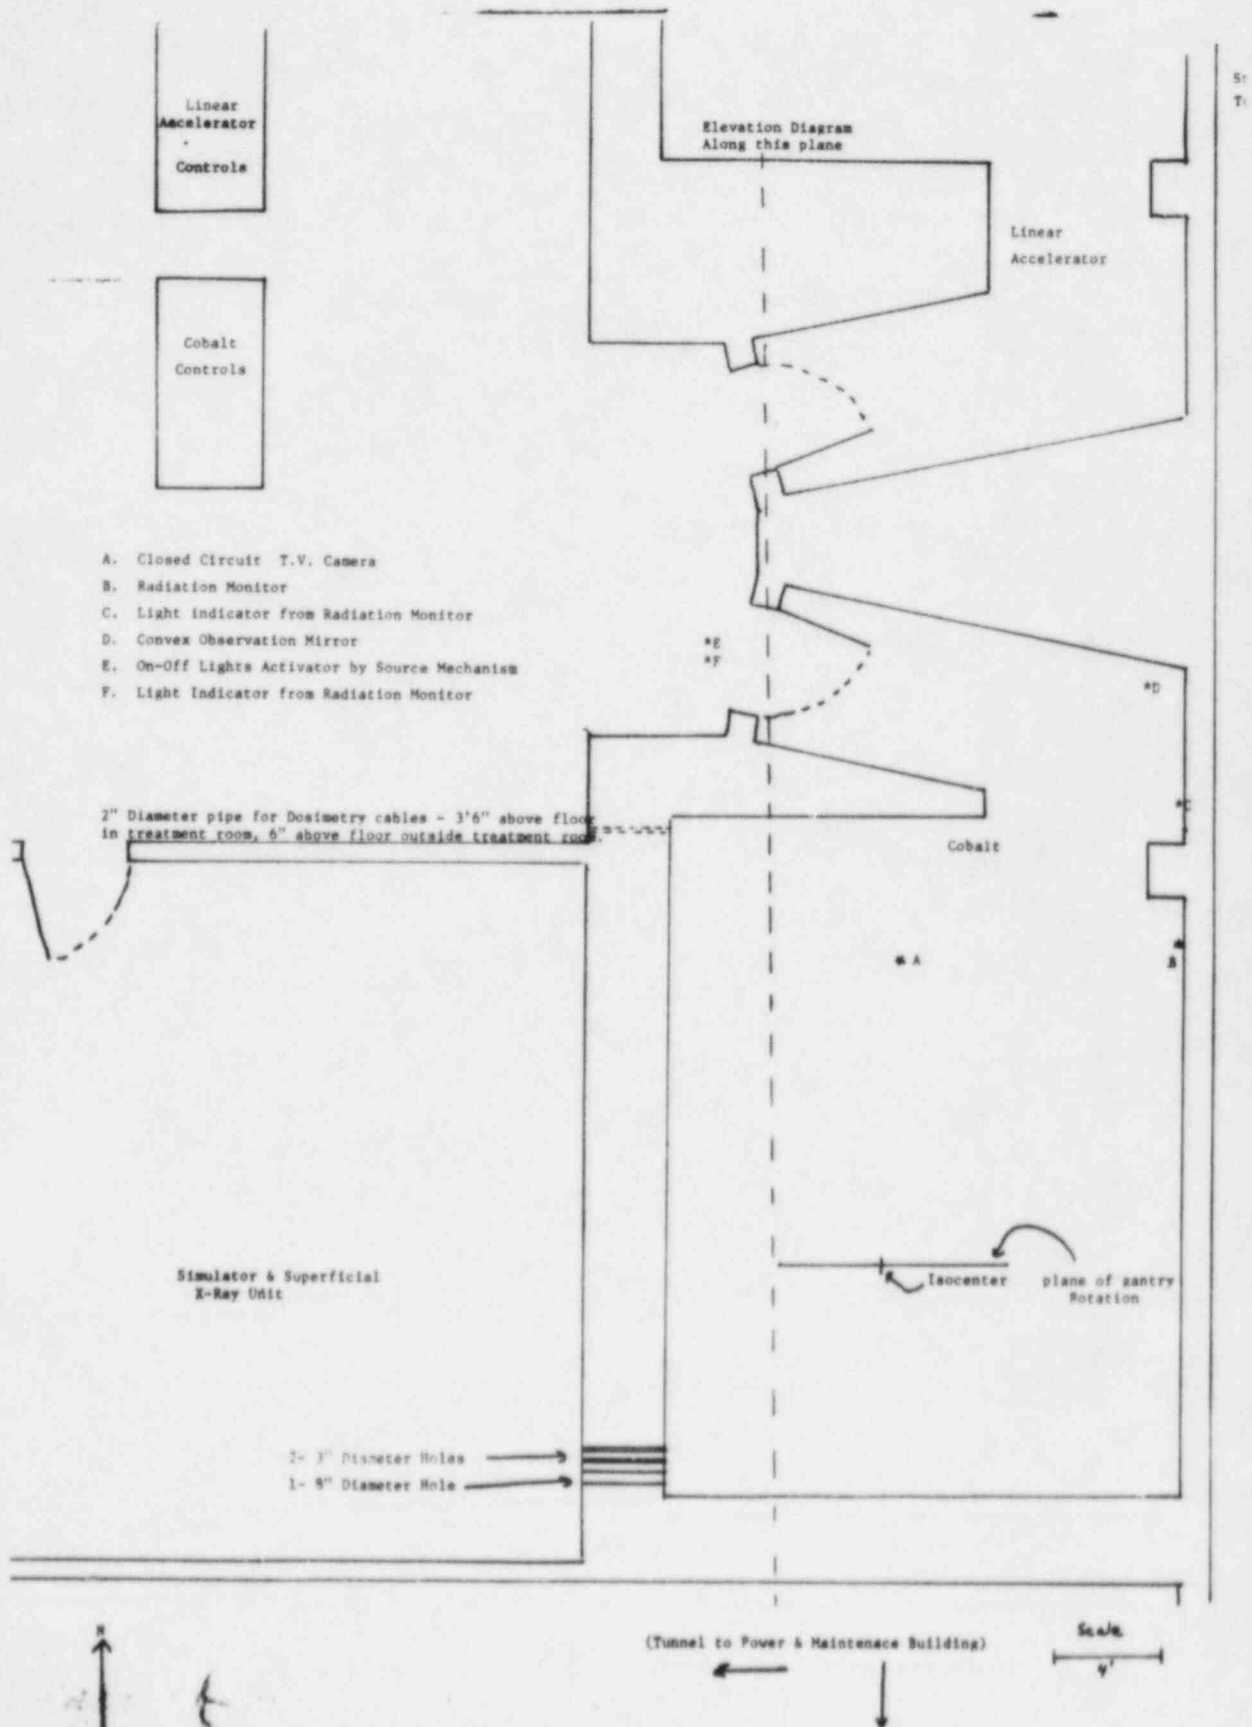

(This area occupied by Central Supplies)

Speckled Area of High Density Concrete  
(200 lbs./Cu. Ft.)

Standard Concrete

Standard Concrete

Tunnel to Power &  
Maintenance Bldg.

Isocenter

A

B (inside)

B (outside)

Door to  
Cobalt

Door to Linear  
Accelerator

Linear  
Accelerator


A - TV Monitor


B - Radiation Monitor

B - 2" Diameter Pipe for Dosimetry Cables

Scale 1" = 1'



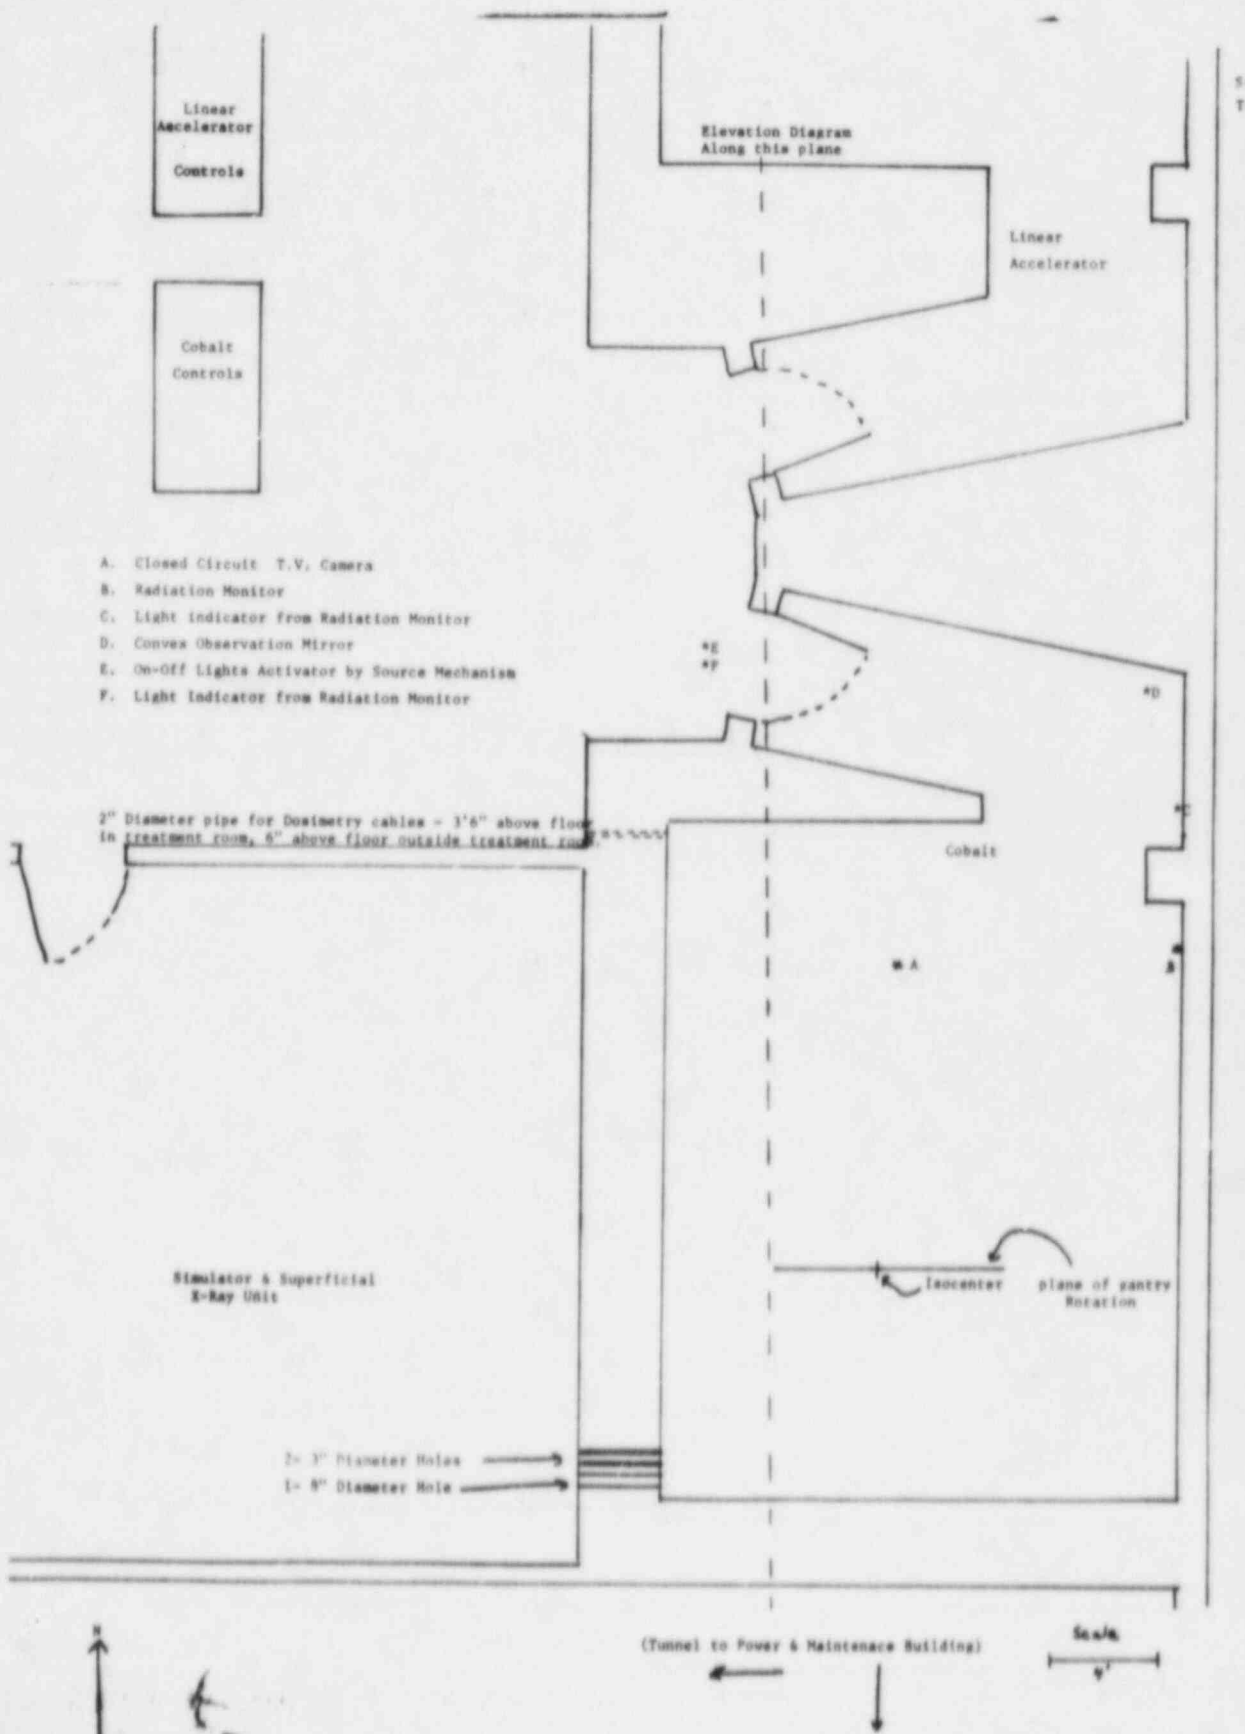

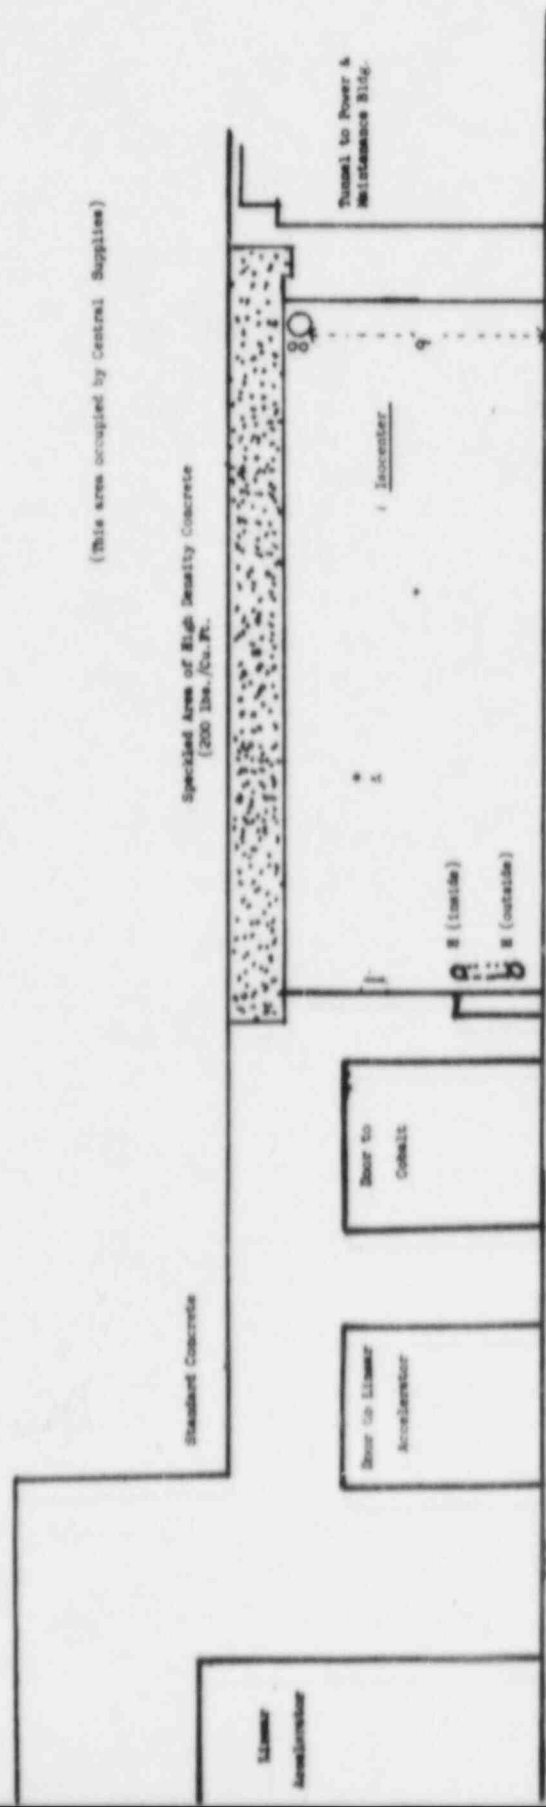

(This area occupied by Central Supplies)

Specified Area of High Density Concrete  
(200 lbs./Cu. Ft.)

Standard Concrete

Standard Concrete

- A - TV Monitor
- B - Radiation Monitor
- E - 2" Diameter Pipe for Dosimetry Cables

Scale 1/2" = 1'

DATE 5/29 - 85

TELEPHONE OR VERBAL CONVERSATION RECORD

TIME 2 ☐ A.M. ☒ P.M.

☐ INCOMING CALL

☒ OUTGOING CALL

☐ VISIT

PERSON CALLING

OFFICE/ADDRESS

PHONE NUMBER | EXTENSION

PERSON CALLED

OFFICE/ADDRESS

PHONE NUMBER | EXTENSION

Keith Jones, Ph.D.

St. John Med. Ctr. Tulsa, OK

918-744-2345

CONVERSATION

SUBJECT

Teletherapy Survey Report

SUMMARY

- 1) Send referenced Teletherapy Head survey report
- 2) " " Facility Sketch
- 3) Change source designation to NPI-20-7000 W  
from NPO-20-7000 W

Licensee will respond ASAP.

MS-15  
5/29  
71

REFERRED TO:

*[Signature]*

MS-15

ACTION REQUESTED

☐ ADVISE ME OF ACTION TAKEN.

INITIALS

*[Signature]*

DATE

5/29

ACTION TAKEN

INITIALS

DATE




UNITED STATES  
NUCLEAR REGULATORY COMMISSION

REGION IV  
611 RYAN PLAZA DRIVE, SUITE 1000  
ARLINGTON, TEXAS 76011

BETWEEN: William O. Miller, Chief  
License Fee Management Branch  
Office of Administration

R. J. Everett, Chief  
Material Radiation Protection Section, TPB,  
DV&TP, RIV

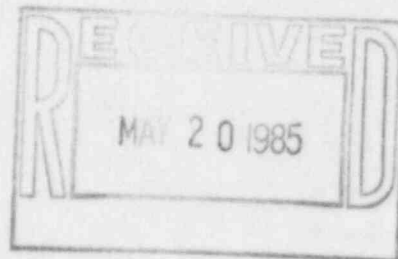

LICENSEE FEE TRANSMITTAL

A. REGION IV

1. APPLICATION ATTACHED

Applicant/Licensee:

Application Dated:

Control No.:

License No.:

St. John Med. Ctr.  
April 26, 1985  
460619  
35-00376-05 (030-11619)

2. FEE ATTACHED

Amount:

Check No.:

3. COMMENTS

Signed

Date

Laura Hurley  
May 6, 1985

02300

B. LICENSEE FEE MANAGEMENT BRANCH

1. Fee Category and Amount:

2. Correct Fee Paid. Application may be processed for:

Amendment ✓

Renewal       

License       

7A FEE EXEMPT 2/86 K.T. Report

Signed

Date

Frances Brown  
5/13/85 5/14/85