

NRC FORM 313M (9-81) 10 CFR 35	U.S. NUCLEAR REGULATORY COMMISSION APPLICATION FOR MATERIALS LICENSE – MEDICAL	Approved by OMB 3150-0041
---	---	------------------------------

INSTRUCTIONS – Complete Items 1 through 26 if this is an initial application or an application for renewal of a license. Use supplemental sheets where necessary. Item 26 must be completed on all applications and signed. Retain one copy. Submit original and one copy of entire application to: Director, Office of Nuclear Materials Safety and Safeguards, U.S. Nuclear Regulatory Commission, Washington, D.C. 20555. Upon approval of this application, the applicant will receive a Materials License. An NRC Materials License is issued in accordance with the general requirements contained in Title 10, Code of Federal Regulations, Part 30, and the Licensee is subject to Title 10, Code of Federal Regulations, Parts 19, 20 and 35 and the license fee provision of Title 10, Code of Federal Regulations, Part 170. The license fee category should be stated in Item 26 and the appropriate fee enclosed.

1.a. NAME AND MAILING ADDRESS OF APPLICANT (institution, firm, clinic, physician, etc.) INCLUDE ZIP CODE BERNARDO A. PUEBLA, M.D. P.O. Box 146 Guayama, Puerto Rico, 00655 TELEPHONE NO.: AREA CODE (809) 864-2010	1.b. STREET ADDRESS(ES) AT WHICH RADIOACTIVE MATERIAL WILL BE USED (If different from 1.a.) INCLUDE ZIP CODE 28W. E. Gonzalez St. Guayama, Puerto Rico, 00655
2. PERSON TO CONTACT REGARDING THIS APPLICATION Bernardo A. Puebla, M.D. TELEPHONE NO.: AREA CODE (809) 864-2010	3. THIS IS AN APPLICATION FOR: (Check appropriate item) a. <input checked="" type="checkbox"/> NEW LICENSE b. <input type="checkbox"/> AMENDMENT TO LICENSE NO. _____ c. <input type="checkbox"/> RENEWAL OF LICENSE NO. _____
4. INDIVIDUAL USERS (Name individuals who will use or directly supervise use of radioactive material. Complete Supplements A and B for each individual.) Bernardo A. Puebla, M.D.	5. RADIATION SAFETY OFFICER (RSO) (Name of person designated as radiation safety officer. If other than individual user, complete resume of training and experience as in Supplement A.) BERNARDO A. PUEBLA, M.D. Santiago Gomez Figueroa, Radiation Physics Consultant

6.a. RADIOACTIVE MATERIAL FOR MEDICAL USE			
RADIOACTIVE MATERIAL LISTED IN:	ITEMS DESIRED "X"	MAXIMUM POSSESSION LIMITS (In millicuries)	<div style="display: flex; justify-content: space-between;"> <div>ADDITIONAL ITEMS:</div> <div> MARK ITEMS DESIRED "X" </div> </div> <div style="text-align: right;">MAXIMUM POSSESSION LIMITS (In millicuries)</div>
10 CFR 31.11 FOR IN VITRO STUDIES			IODINE-131 AS IODIDE FOR TREATMENT OF HYPERTHYROIDISM
10 CFR 35.100, SCHEDULE A, GROUP I		AS NEEDED	PHOSPHORUS-32 AS SOLUBLE PHOSPHATE FOR TREATMENT OF POLYCYTHEMIA VERA, LEUKEMIA AND BONE METASTASES
10 CFR 35.100, SCHEDULE A, GROUP II		AS NEEDED	PHOSPHORUS-32 AS COLLOIDAL CHROMIC PHOSPHATE FOR INTRACAVITARY TREATMENT OF MALIGNANT EFFUSIONS.
10 CFR 35.100, SCHEDULE A, GROUP III			GOLD-198 AS COLLOID FOR INTRACAVITARY TREATMENT OF MALIGNANT EFFUSIONS.
10 CFR 35.100, SCHEDULE A, GROUP IV		AS NEEDED	IODINE-131 AS IODIDE FOR TREATMENT OF THYROID CARCINOMA
10 CFR 35.100, SCHEDULE A, GROUP V		AS NEEDED	XENON-133 AS GAS OR GAS IN SALINE FOR BLOOD FLOW STUDIES AND PULMONARY FUNCTION STUDIES.
10 CFR 35.100, SCHEDULE A, GROUP VI	X	125	

6.b. RADIOACTIVE MATERIAL FOR USES NOT LISTED IN ITEM 6.a. (Sealed sources up to 3 mCi used for calibration and reference standards are authorized under Section 35.14(d), 10 CFR Part 35, and NEED NOT BE LISTED.)			
ELEMENT AND MASS NUMBER	CHEMICAL AND/OR PHYSICAL FORM	MAXIMUM NUMBER OF MILLICURIES OF EACH FORM	DESCRIBE PURPOSE OF USE
Sr-90/Y-90	Sealed Source New England Nuclear Model NE-1 Eye Therapy Source	100	Human use: Treatment of superficial eye conditions

NRC (9-8)
 8512020144 851003
 REG2 LIC30
 52-23097-01 PDR

License Fee Information
 on Next Page

50695
 8/13/85
 21097
 010-28851

INFORMATION REQUIRED FOR ITEMS 7 THROUGH 23

For Items 7 through 23, check the appropriate box(es) and submit a detailed description of all the requested information. Begin each item on a separate sheet. Identify the item number and the date of the application in the lower right corner of each page. If you indicate that an appendix to the medical licensing guide will be followed, do not submit the pages, but specify the revision number and date of the referenced guide: Regulatory Guide 10.8, Rev. _____ Date: _____

7. MEDICAL ISOTOPES COMMITTEE N/A		15. GENERAL RULES FOR THE SAFE USE OF RADIOACTIVE MATERIAL (Check One) N/A	
Names and Specialties Attached; and		Appendix G Rules Followed; or	
Duties as in Appendix B; or _____ (Check One)		Equivalent Rules Attached	
Equivalent Duties Attached		16. EMERGENCY PROCEDURES (Check One)	
8. TRAINING AND EXPERIENCE		Appendix H Procedures Followed; or	
<input checked="" type="checkbox"/>	Supplements A & B Attached for Each Individual User; and	<input checked="" type="checkbox"/>	Equivalent Procedures Attached See Annex III
<input checked="" type="checkbox"/>	Supplement A Attached for RSO.	17. AREA SURVEY PROCEDURES (Check One) N/A	
9. INSTRUMENTATION (Check One)		Appendix I Procedures Followed; or	
<input checked="" type="checkbox"/>	Appendix C Form Attached; or See Annex I	Equivalent Procedures Attached	
List by Name and Model Number		18. WASTE DISPOSAL (Check One)	
10. CALIBRATION OF INSTRUMENTS		Appendix J Form Attached; or	
<input checked="" type="checkbox"/>	Appendix D Procedures Followed for Survey Instruments; or See Annex I _____ (Check One)	<input checked="" type="checkbox"/>	Equivalent Information Attached See Annex III
Equivalent Procedures Attached; and		19. THERAPEUTIC USE OF RADIOPHARMACEUTICALS (Check One) N/A	
Appendix D Procedures Followed for Dose Calibrator; or _____ (Check One)		Appendix K Procedures Followed; or	
Equivalent Procedures Attached		Equivalent Procedures Attached	
11. FACILITIES AND EQUIPMENT		20. THERAPEUTIC USE OF SEALED SOURCES	
<input checked="" type="checkbox"/>	Description and Diagram Attached See Annex II	<input checked="" type="checkbox"/>	Detailed Information Attached; and
12. PERSONNEL TRAINING PROGRAM		Appendix L Procedures Followed; or _____ (Check One)	
<input checked="" type="checkbox"/>	Description of Training Attached See Annex III	<input checked="" type="checkbox"/>	Equivalent Procedures Attached See Annex III
13. PROCEDURES FOR ORDERING AND RECEIVING RADIOACTIVE MATERIAL N/A		21. PROCEDURES AND PRECAUTIONS FOR USE OF RADIOACTIVE GASES (e.g., Xenon - 133) N/A	
Detailed Information Attached		Detailed Information Attached	
14. PROCEDURES FOR SAFELY OPENING PACKAGES CONTAINING RADIOACTIVE MATERIALS (Check One) N/A		22. PROCEDURES AND PRECAUTIONS FOR USE OF RADIOACTIVE MATERIAL IN ANIMALS N/A	
Appendix F Procedures Followed; or		Detailed Information Attached	
Equivalent Procedures Attached		23. PROCEDURES AND PRECAUTIONS FOR USE OF RADIOACTIVE MATERIAL SPECIFIED IN ITEM 6.b	
		<input checked="" type="checkbox"/>	Detailed Information Attached See Annex III

24. PERSONNEL MONITORING DEVICES

	TYPE <small>(Check appropriate box)</small>	SUPPLIER	EXCHANGE FREQUENCY	
a. WHOLE BODY	<input type="checkbox"/> FILM			
	<input type="checkbox"/> TLD			
	<input type="checkbox"/> OTHER (Specify)	<u>Remark:</u> At the present time I do not feel it is necessary to wear a personnel monitoring device, since the number of cases treated with the Sr-90 Eye Applicator in my private practice has not been greater than ten patients per month. In the event that this situation changes, and then additional cases are treated, i.e. 20 or more patients per month, the steps towards the use of personnel monitoring devices will be as follows:		
<input type="checkbox"/> FILM				
b. FINGER	<input type="checkbox"/> TLD			
	<input type="checkbox"/> OTHER (Specify)			
	c. WRIST	<input type="checkbox"/> FILM		
<input type="checkbox"/> TLD				
<input type="checkbox"/> OTHER (Specify)				
d. OTHER (Specify)				

- a. Organization supplying the monitoring devices:
Landauer Jr. or equivalent organization
- b. Type of monitoring devices:
Whole Body and Finger Badges
- c. Frequency : Monthly

Aug-2-II

Applicant.....
Check No. <i>152</i>
Amount For..... <i>\$580.00</i>
Type of Fee..... <i>app</i>
Date Check Recd..... <i>8/19/85</i>
Received By..... <i>J. A. G. Lino</i>

25. FOR PRIVATE PRACTICE APPLICANTS ONLY

a. HOSPITAL AGREEING TO ACCEPT PATIENTS CONTAINING RADIOACTIVE MATERIAL		b. ATTACH A COPY OF THE AGREEMENT LETTER SIGNED BY THE HOSPITAL ADMINISTRATOR.
NAME OF HOSPITAL <i>N/A</i>		c. WHEN REQUESTING THERAPY PROCEDURES, ATTACH A COPY OF RADIATION SAFETY PRECAUTIONS TO BE TAKEN AND LIST AVAILABLE RADIATION DETECTION INSTRUMENTS.
MAILING ADDRESS		
CITY	STATE ZIP CODE	

26. CERTIFICATE

(This item must be completed by applicant)

The applicant and any official executing this certificate on behalf of the applicant named in Item 1a certify that this application is prepared in conformity with Title 10, Code of Federal Regulations, Parts 30 and 35, and that all information contained herein, including any supplements attached hereto, is true and correct to the best of our knowledge and belief.

a. LICENSE FEE REQUIRED <i>(See Section 170.31, 10 CFR 170)</i>	b. APPLICANT OR CERTIFYING OFFICIAL (Signature) <div style="text-align: center;"><i>[Signature]</i></div>
(1) LICENSE FEE CATEGORY: <i>7C</i>	(1) NAME (Type of Print) <i>Bernardo A. Puebla, M.D.</i>
(2) LICENSE FEE ENCLOSED: \$ <i>580.00</i>	(2) TITLE <i>Ophthalmologist</i>
	c. DATE <i>June 12, 1985</i>

PRIVACY ACT STATEMENT

Pursuant to 5 U.S.C. 552a(e)(3), enacted into law by section 3 of the Privacy Act of 1974 (Public Law 93-579), the following statement is furnished to individuals who supply information to the Nuclear Regulatory Commission on NRC Form 313M. This information is maintained in a system of records designated as NRC-3 and described at 40 Federal Register 45334 (October 1, 1975).

1. **AUTHORITY** Sections 81 and 161(b) of the Atomic Energy Act of 1954, as amended (42 U.S.C. 2111 and 2201(b)).
2. **PRINCIPAL PURPOSE(S)** The information is evaluated by the NRC staff pursuant to the criteria set forth in 10 CFR Parts 30-36 to determine whether the application meets the requirements of the Atomic Energy Act of 1954, as amended, and the Commission's regulations, for the issuance of a radioactive material license or amendment thereof.
3. **ROUTINE USES** The information may be used: (a) to provide records to State health departments for their information and use; and (b) to provide information to Federal, State, and local health officials and other persons in the event of incident or exposure, for their information, investigation, and protection of the public health and safety. The information may also be disclosed to appropriate Federal, State, and local agencies in the event that the information indicates a violation or potential violation of law and in the course of an administrative or judicial proceeding. In addition, this information may be transferred to an appropriate Federal, State, or local agency to the extent relevant and necessary for a NRC decision or to an appropriate Federal agency to the extent relevant and necessary for that agency's decision about you. A copy of the license issued will routinely be placed in the NRC's Public Document Room, 1717 H Street, N.W., Washington, D.C.
4. **WHETHER DISCLOSURE IS MANDATORY OR VOLUNTARY AND EFFECT ON INDIVIDUAL OF NOT PROVIDING INFORMATION** Disclosure of the requested information is voluntary. If the requested information is not furnished, however, the application for radioactive material license, or amendment thereof, will not be processed.
5. **SYSTEM MANAGER(S) AND ADDRESS** Director, Division of Fuel Cycle and Material Safety, Office of Nuclear Material Safety and Safeguards, U.S. Nuclear Regulatory Commission, Washington, D.C. 20555.

Items 4,5 and 6b

1. Supplement A and B (Dr. Bernardo A. Puebla)
2. Supplement A and Resumé (Santiago Gómez Figueros)
3. New England Nuclear Bulletin on NEN-Model NB-1
Eye Therapy Source

TRAINING AND EXPERIENCE
AUTHORIZED USER OR RADIATION SAFETY OFFICER

1. NAME OF AUTHORIZED USER OR RADIATION SAFETY OFFICER BERNARDO A. PUEBLA, M.D.		2. STATE OR TERRITORY IN WHICH LICENSED TO PRACTICE MEDICINE P.R.		
3. CERTIFICATION				
SPECIALTY BOARD A	CATEGORY B	MONTH AND YEAR CERTIFIED C		
Candidate American Board of Ophthalmology	Residency University of Puerto Rico (UPR) School of Medicine	June, 1983		
4. TRAINING RECEIVED IN BASIC RADIOISOTOPE HANDLING TECHNIQUES				
FIELD OF TRAINING A	LOCATION AND DATE(S) OF TRAINING B	TYPE AND LENGTH OF TRAINING		
		LECTURE/ LABORATORY COURSES (Hours) C	SUPERVISED LABORATORY EXPERIENCE (Hours) D	
a. RADIATION PHYSICS AND INSTRUMENTATION	UPR-School of Medicine Ophthalmology Department San Juan, Puerto Rico August 8, 1981 - February 11, 1982	8	3	
b. RADIATION PROTECTION	Same as above	10	2	
c. MATHEMATICS PERTAINING TO THE USE AND MEASUREMENT OF RADIOACTIVITY	Same as above	5	-	
d. RADIATION BIOLOGY	Same as above	10	2	
e. RADIOPHARMACEUTICAL CHEMISTRY	--	-	-	
5. EXPERIENCE WITH RADIATION. (Actual use of Radioisotopes or Equivalent Experience)				
ISOTOPE	MAXIMUM AMOUNT	WHERE EXPERIENCE WAS GAINED	DURATION OF EXPERIENCE	TYPE OF USE
Sr-90	50 mCi	Medical Center, San Juan P.R.	1980-1983	Therapy
Sr-90	50 mCi	V.A. Hospital, San Juan P.R.	1980-1983	Therapy

PRECEPTOR STATEMENT

Supplement B must be completed by the applicant physician's preceptor. If more than one preceptor is necessary to document experience, obtain a separate statement from each.

1. APPLICANT PHYSICIAN'S NAME AND ADDRESS

FULL NAME

BERNARDO A. PUEBLA, M.D.

STREET ADDRESS

28 W E. Gonzalez St.
Guayama, P.R. 00655

CITY

Guayama

STATE

P.R.

ZIP CODE

00655

KEY TO COLUMN C

PERSONAL PARTICIPATION SHOULD CONSIST OF:

- 1-Supervised examination of patients to determine the suitability for radioisotope diagnosis and/or treatment and recommendation for prescribed dosage.
- 2-Collaboration in dose calibration and actual administration of dose to the patient including calculation of the radiation dose, related measurements and plotting of data.
- 3-Adequate period of training to enable physician to manage radioactive patients and follow patients through diagnosis and/or course of treatment.

2. CLINICAL TRAINING AND EXPERIENCE OF ABOVE NAMED PHYSICIAN

ISOTOPE A	CONDITIONS DIAGNOSED OR TREATED B	NUMBER OF CASES INVOLVING PERSONAL PARTICIPATION C	COMMENTS (Additional information or comments may be submitted in duplicate on separate sheets.) D
I-131 or I-125	DIAGNOSIS OF THYROID FUNCTION		
	DETERMINATION OF BLOOD AND BLOOD PLASMA VOLUME		
	LIVER FUNCTION STUDIES		
	FAT ABSORPTION STUDIES		
	KIDNEY FUNCTION STUDIES		
	IN VITRO STUDIES		
OTHER			
I-125	DETECTION OF THROMBOSIS		
I-131	THYROID IMAGING		
P-32	EYE TUMOR LOCALIZATION		
Se-75	PANCREAS IMAGING		
Yb-169	CISTERNOGRAPHY		
Xe-133	BLOOD FLOW STUDIES AND PULMONARY FUNCTION STUDIES		
OTHER			
Tc-99m	BRAIN IMAGING		
	CARDIAC IMAGING		
	THYROID IMAGING		
	SALIVARY GLAND IMAGING		
	BLOOD POOL IMAGING		
	PLACENTA LOCALIZATION		
	LIVER AND SPLEEN IMAGING		
	LUNG IMAGING		
	BONE IMAGING		
OTHER			

PRECEPTOR STATEMENT (Continued)

2. CLINICAL TRAINING AND EXPERIENCE OF ABOVE NAMED PHYSICIAN (Continued)

ISOTOPE A	CONDITIONS DIAGNOSED OR TREATED B	NUMBER OF CASES INVOLVING PERSONAL PARTICIPATION C	COMMENTS (Additional information or comments may be submitted in duplicate on separate sheets.) D
P-32 (Soluble)	TREATMENT OF POLYCYTHEMIA VERA, LEUKEMIA, AND BONE METASTASES		<p>As routine all cases of Pterygium Surgery in our Institution receive beta radiation to minimize recurrences. Approximate dose given: 2000 rads</p> <p>Following are three cases of patients treated by Dr. Bernardo A. Puebla during his Residency:</p> <p>1. Carmen Vega Osorio (9-10-81) Dose: 2000 rads</p> <p>2. Francisca Sánchez Corchado (9-21-81) Dose: 2000 rads</p> <p>3. Luisa Cuevas Castro (6-3-81) Dose: 2000 rads</p>
P-32 (Colloidal)	INTRACAVITARY TREATMENT		
I-131	TREATMENT OF THYROID CARCINOMA		
	TREATMENT OF HYPERTHYROIDISM		
Au-198	INTRACAVITARY TREATMENT		
Co-60 or Cs-137	INTERSTITIAL TREATMENT		
	INTRACAVITARY TREATMENT		
I-125 or Ir-192	INTERSTITIAL TREATMENT		
Co-60 or Cs-137	TELE THERAPY TREATMENT		
Sr-90	TREATMENT OF EYE DISEASE	150	
	RADIOPHARMACEUTICAL PREPARATION		
Mo-99/ Tc-99m	GENERATOR		
Sn-113/ In-113m	GENERATOR		
Tc-99m	REAGENT KITS		
Other			

3. DATES AND TOTAL NUMBER OF HOURS RECEIVED IN CLINICAL RADIOISOTOPE TRAINING

On the job training during Residency from 1980 to 1983

4. THE TRAINING AND EXPERIENCE INDICATED ABOVE WAS OBTAINED UNDER THE SUPERVISION OF:

a. NAME OF SUPERVISOR

Manuel N. Miranda, M.D.

b. NAME OF INSTITUTION

UPR-School of Medicine

c. MAILING ADDRESS

G.P.O. Box 5067

d. CITY

San Juan, P.R. 00936

5. MATERIALS LICENSE NUMBER(S)

52-01946-07

6. PRECEPTOR'S SIGNATURE

Manuel N. Miranda

7. PRECEPTOR'S NAME (Please type or print)

MANUEL N. MIRANDA, M.D.

8. DATE

June 6, 1985

TRAINING AND EXPERIENCE
AUTHORIZED USER OR RADIATION SAFETY OFFICER

1. NAME OF AUTHORIZED USER OR RADIATION SAFETY OFFICER SANTIAGO GOMEZ FIGUEROA (see Resume)	2. STATE OR TERRITORY IN WHICH LICENSED TO PRACTICE MEDICINE
--	--

3. CERTIFICATION		
SPECIALTY BOARD A	CATEGORY B	MONTH AND YEAR CERTIFIED C
	N/A	

4. TRAINING RECEIVED IN BASIC RADIOISOTOPE HANDLING TECHNIQUES			
FIELD OF TRAINING A	LOCATION AND DATE(S) OF TRAINING B	TYPE AND LENGTH OF TRAINING	
		LECTURE/ LABORATORY COURSES (Hours) C	SUPERVISED LABORATORY EXPERIENCE (Hours) D
a. RADIATION PHYSICS AND INSTRUMENTATION	Puerto Rico Nuclear Center (PRNC) and University of P.R. (UPR)-School of Medicine, S.J. PR. 1972	200	150
b. RADIATION PROTECTION	PRNC and UPR-School of Medicine 1972 - 73	200	150
c. MATHEMATICS PERTAINING TO THE USE AND MEASUREMENT OF RADIOACTIVITY	PRNC and UPR-School of Medicine 1972 - 73	200	150
d. RADIATION BIOLOGY	PRNC and UPR-School of Medicine 1973	150	100
e. RADIOPHARMACEUTICAL CHEMISTRY	PRNC and UPR-School of Medicine 1973	50	50

5. EXPERIENCE WITH RADIATION. (Actual use of Radioisotopes or Equivalent Experience)				
ISOTOPE	MAXIMUM AMOUNT	WHERE EXPERIENCE WAS GAINED	DURATION OF EXPERIENCE	TYPE OF USE
Co-60	4000 Ci	PRNC and UPR-Medical Sciences Campus (MSC) San Juan, P.R.	8 years	Res. Irradiator
Cs-137	0.8 Ci	PRNC and MSC	10 years	Therapy Sealed Sources
Co-60	5000 Ci	PRNC & Univ. Dist. Hosp. V.A. Hospital, San Juan, PR.	10 years 3 years	Therapy Units Therapy Units
H-3	2300 Ci	TII Ind. Inc.-Tos Alts, PR.	6 years	Electronic Tubes
				Production.

Cont... #5 EXPERIENCE WITH RADIATION

Short-lived radionuclides	PRNC-MSD, V.A. Hospital and Private Nuc.Med.Lab., S.J.	10 years	Diagnostic
I-131 100 mCi/treatment	University District Hospital	10 years	Therapy
Sr-90 100 mCi/Applicat.	Ophthalmologists Private Offices	8 years	Therapy

CURRICULUM VITAE (RESUME)

Name:

SANTIAGO GOMEZ

Residence and Mailing Address:

1821 Colonia St.
College Park
Río Piedras, Puerto Rico (00921)
Phone (809) 751-0042

Business Address:

UPR- Medical Sciences Campus
Health Physics Office
Bio-Medical Building (R-180)
Caparra Heights Station
San Juan, Puerto Rico (00935)

Phone (809) 767-0396

Marital Status:

Married, 2 children

Education:

Universidad Nacional and Instituto de la
Salle
Bogotá, Colombia - 1954-1958 (Sciences)
B.S.

Cath. University of America - Washington-
1960-62 (Physics) - M.S.

Specialization:

- University of Puerto Rico
(Medical Sciences Campus) - San Juan
1972 - 1973 (Radiological Health) M.S.

Content of the courses:

- a) Principles of Radiation Physics
and Radiation Detection.
 - b) Principles and practices of
radiation protection.
 - c) Radioactivity measurement standarization
and monitoring techniques and
instruments.
 - d) Mathematics and calculations basic
to the use and measurement of
radioactivity.
 - e) Biological effects of radiation.
- MIT - Boston, Massachusetts - August
1983 Summer Course on:
"Non-Ionizing Radiations: Biophysical
and Biological Applications and
Hazards in Medicine and Industry ".

Positions Held:

- Professor of physics at the School of Engineering - Univ. Industrial de Santander - Bucaramanga-Colombia 1963-1971
- Teacher and coordinator of courses on applied radiation physics at the school of Medicine - Univ. Industrial de Santander - Bucaramanga - Colombia 1973-1974
- Professor of Radiation Detection and Radiological Health courses at the School of Medicine U.P.R., San Juan, P.R. 1974-1975
- Head of the Health and Safety Division, Río Piedras Operations, Center for Energy and Environment Research 1974-1978
- Radiation Protection Officer
UPR- Medical Sciences Campus
NRC Broad Scope Licensee
San Juan, Puerto Rico
1978 - up to date
- Radiation Physics Consultant
TII Industries Inc., Toa Alta, P.R.
(multicuries use of H-3 for electronic tubes production)
1975- up to date (part-time)

Experience with Radiation:

- Research on plantains and mangoes preservation by gamma radiation -PRNC 1972
- Isodose curves mapping on a phantom exposed to a Co-60 radiation field using TLD microrods PRNC - 1973
- The solution of a Dosimetry Problem caused by a Mercury Shutter.
Published in Phy. Med. and Biol., 1976
- Radiation dose to personnel during routine Nuclear Medicine Analysis
PRNC - 1976
- Tutoring undergraduate students users of a Co-60 Irradiator (approx. 2000 Ci)
PRNC- 1975, up to date.

- Radiological Health Services provided to UPR-Medical Sciences Campus, TII Industries Inc., three Nuclear Medicine laboratories and six private Industrial and Medical Laboratories, including:
 - a) Urine Analysis for H-3
 - b) Smears and surveys
 - c) Leak test to Co-60 Teletherapy Units (5000 Ci), Cs-137 needles and tubes (350 mCi), Sr-90 Eye Applicators (100 mCi), Ir-192 (Seeds) 100 mCi, Ni-63 Sealed Sources (15 mCi)
 - d) Indoctrination on Radiation Protection to new personnel
 - e) Radiation detection instruments calibration
 - f) Radwaste collection and disposal
 - g) Consultant Services on NRC License Applications.

Membership Professional

Societies:

Asociación Colombiana para el Avance de la Ciencia.

Health Physics Society, Puerto Rico Chapter

Sociedad de Medicina Nuclear de Puerto Rico

Health Physics Society, plenary Member
American Association of Physics Teachers.

Additional Qualifications:

- a) Fellowships: UNESCO - Amsterdam 1965-1966
National Sciences Foundation - Rutgers University - Summer 1962
OAS - San Juan, Puerto Rico 1972-1973
National Safety Council - Philadelphia 1975
- b) Achievement: ERDA Safety Award to PRNC 1975, 1976, 1977, 1978
- c) NRC License No. 52-17420-01 for Leak Testing of Sealed Sources
- d) Comprehensive Organization of the UPR- Medical Sciences Campus Radiation Protection Program including elaboration of the Broad Scope, Teletherapy Unit and Gamma Irradiator NRC License Applications.

NEN New England Nuclear

Model NB-1 Eye Therapy Source

Ophthalmic Beta Radiation Applicator

New England Nuclear's NB-1 Eye Therapy Source is designed for use in the treatment of superficial eye conditions that respond to beta radiation. Conditions which may respond well include vernal conjunctivitis, corneal vascularization, and keratitis. This source also offers a convenient means of treatment of lesions such as pterygia and papillomas.

DESCRIPTION

Strontium-90 and yttrium-90 in secular equilibrium are uniformly dispersed in an inert matrix which, in turn, is encapsulated in stainless steel with a welded closure. The source has an active diameter of approximately 8.7mm, with an overall diameter of 10.3mm, and is mounted with a swivel joint at the end of a 16cm handle.

Uniformity of the radionuclide deposit is demonstrated by autoradiography. The source contains 100mCi of ^{90}Sr , and delivers approximately 60 rads per second. Each unit is supplied with calibration data traceable to the National Bureau of Standards.

ACCESSORIES FURNISHED WITH THE SOURCE

To protect the therapist's hand during use, each source is fitted with a 5mm thick lucite beta backscatter shield that slides along the handle.

Four Castroviejo collimating masks—designed to confine beta radiation to the selected area of the eye and to protect surrounding tissue. The masks accomplish confinement by permitting 100% transmission through the aperture, and restricting radiation to surrounding tissue. Two masks permit irradiation of circular areas, and two irradiate limbus-shaped areas.

Forceps are provided for ease in affixing and detaching the collimators.

REGISTERED SOURCE SIMPLIFIES LICENSING PROCEDURE

Specific USNRC or Agreement State license authorization is required for possession of this medical device. This unit is registered, however, with the USNRC and, through reciprocity laws, with Agreement States. Because complete manufacturing information is on file under NEN's model number NB-1, those making application for a license need only specify this model number.

ORDERING INFORMATION

MODEL NO. NB-1 Eye Therapy Source
100mCi $^{90}\text{Sr}/^{90}\text{Y}$

Approximate dose rate 60 rad/sec. surface contact dose. Supplied with lucite beta shield, four Castroviejo collimating masks, forceps, detailed instruction manual.

Catalog No. NER-8090

For convenient storage, each source is furnished in a wooden case fitted with stainless steel and tungsten shielding.

New England Nuclear is the world's leading manufacturer of radioactive materials for research and a principal supplier of radio-pharmaceuticals. You can rely on NEN quality—there is no competitive equal.

For further information call or write NEN Technical Services Department.

LIMITED WARRANTY

New England Nuclear (NEN) warrants that, at the time of shipment, the products sold by it are free from defects in material and workmanship and conform to specifications which accompany the product. **NEN makes no other warranty, express or implied, with respect to the products, including any warranty of merchantability or fitness for any particular purpose.** Because of the inherent susceptibility to deterioration of radioactive products, notification of any breach of warranty must be made within 60 days of receipt or within the half-life of the radioisotope contained in the product, whichever period is shorter, unless otherwise provided in writing by NEN. No claim shall be honored if the customer fails to so notify NEN within the period specified. **The sole and exclusive remedy of the customer for any liability of NEN of any kind including liability based upon warranty (express or implied, whether contained herein or elsewhere), strict liability, contract or otherwise is limited to the replacement of the goods or the refund of the invoice price of the goods. NEN shall not in any case be liable for special, incidental or consequential damages of any kind.**



New England Nuclear

Europe

NEN Chemicals GmbH
D-6072 Dreieich, W. Germany
Postfach 401240, Tel. (06103) 85034
Order Entry: (06103) 81011
Telex: 4-17999-NEN D

601 Treble Cove Rd., North Billerica, MA 01862

CALL TOLL-FREE: 800-225-1572 Telex: 94-0996
(In Massachusetts and International: 617-667-9531)

Canada

NEN Canada
2453 46th Avenue
Lachine, Que. H8T 3C9
Tel. 514-636-4971
Telex: 05-821808

ANNEX I

(Items 9 and 10)

1. Accessibility to a properly calibrated G.M. Survey Meter.

In case of emergency, during leak testing procedures, receiving the Applicator from the manufacturer, packing and delivery of the Applicator for repair or maintenance services or in any other case requiring radiation levels determination, arrangements have been made with my Radiation Physics Consultant to ensure access to a recently calibrated G.M. survey meter. Besides that I want him to perform routine radiation levels evaluation around the storage location of the source at the time of performing the biannual leak test.

2. Calibration of the instrument.

Calibration of the Radiation Survey Meter will be performed according to the procedures adopted by the UPR-Medical Sciences Campus - NRC License No. 52-01946-07

A N N E X I I

(Item 11)

The Layout Diagram of the Office facilities describes the location where the source will be stored.


For security purposes, the Sr-90 Ophthalmic Applicator will be stored in a keyed cabinet.

Keys will be kept on hand by the user, Dr. Bernardo A. Puebla, at his desk in the Office.

(Please see the Layout Diagram)

BERNARDO A. PUEBLA, M.D. OFFICE LAYOUT DIAGRAM

SCALE: 1" = 5'-0"

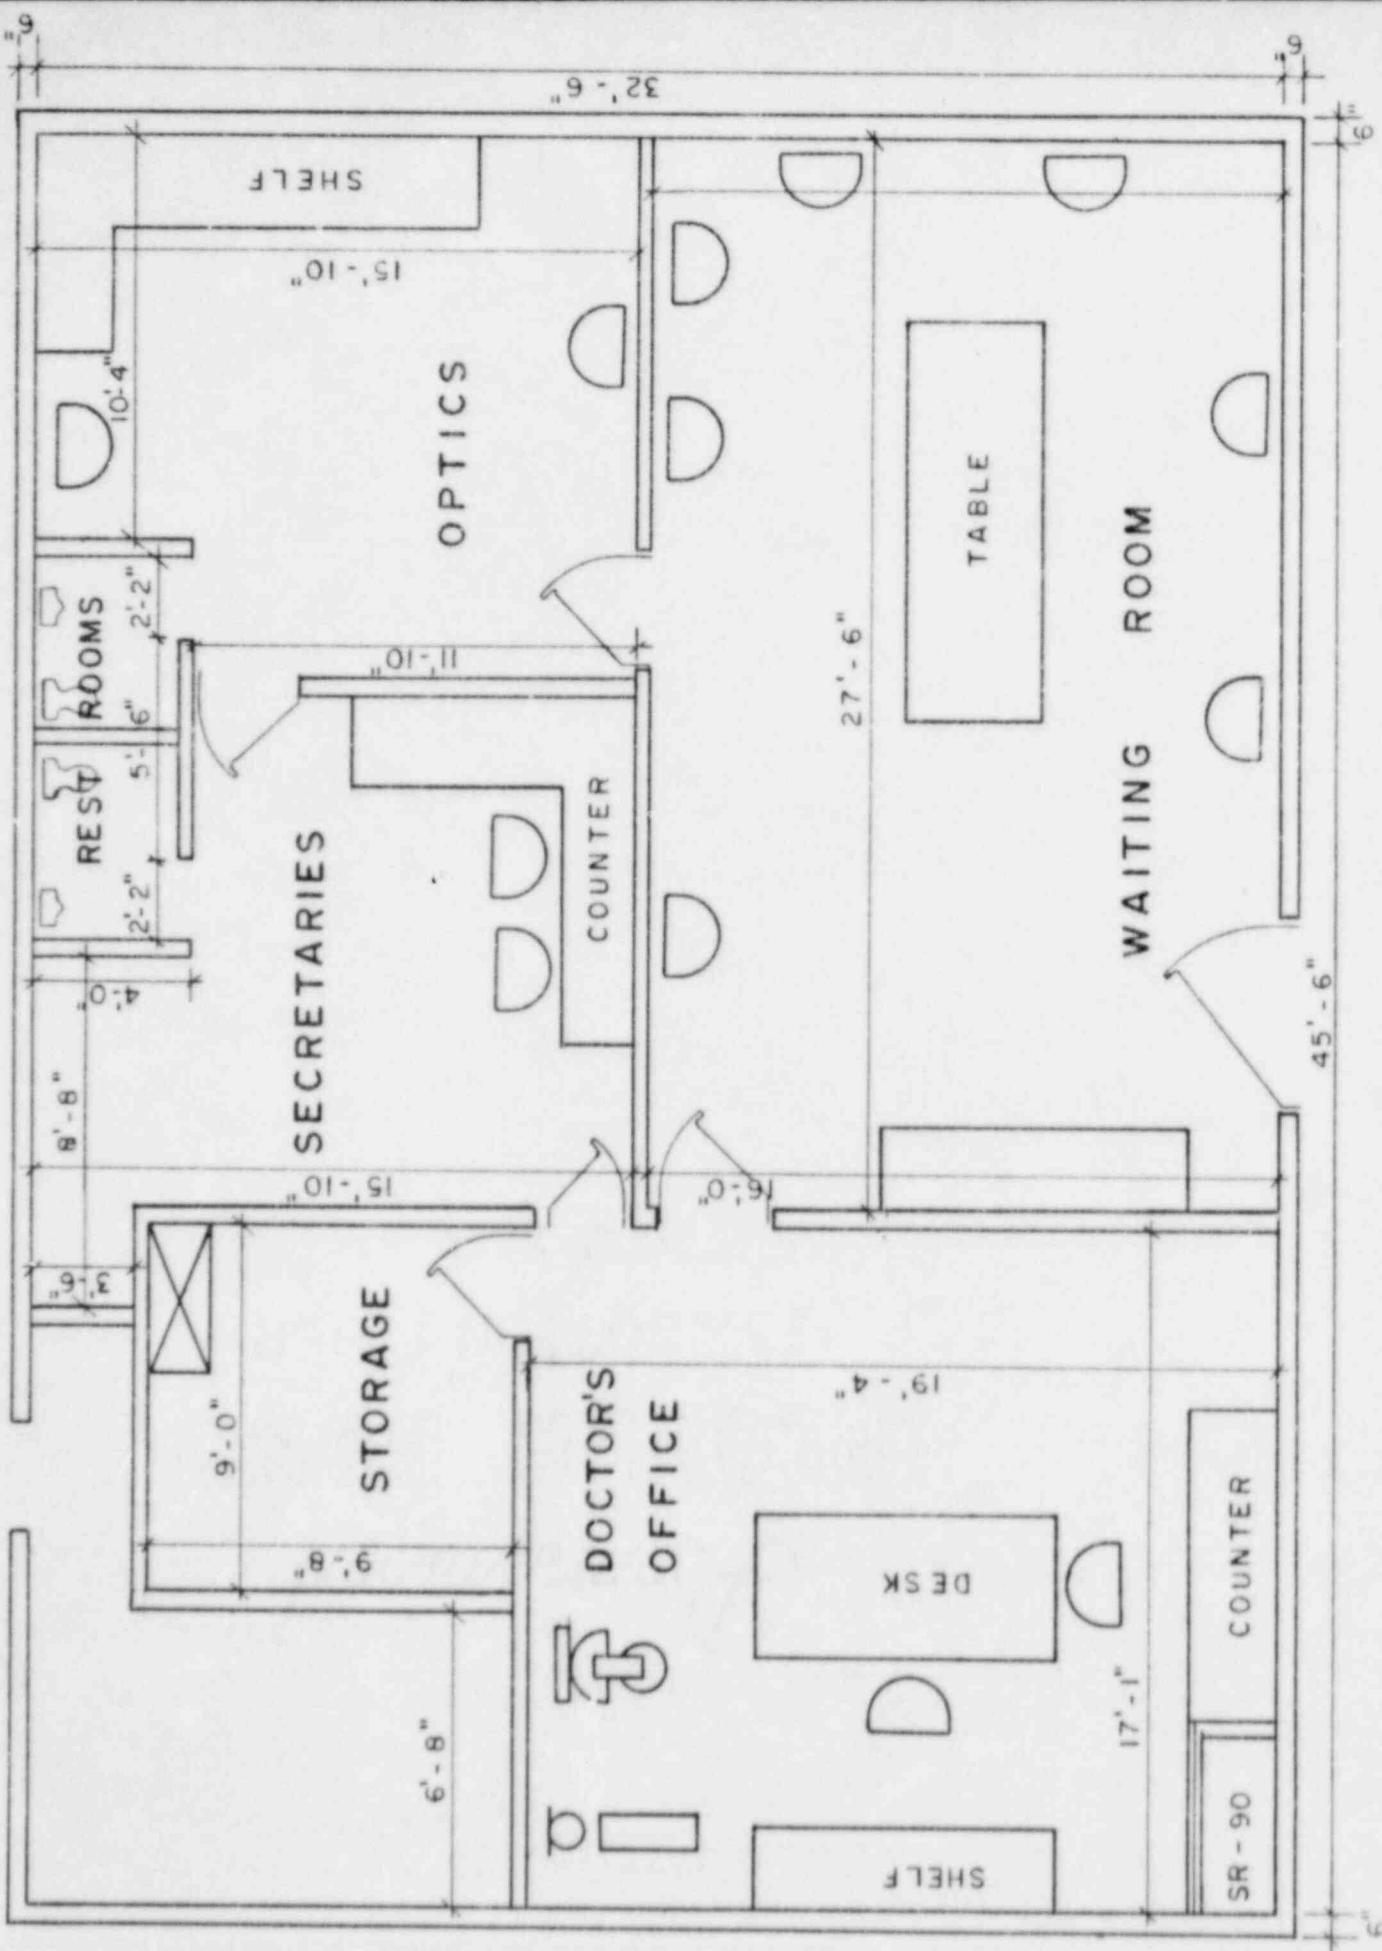

A N N E X I I I

(Items 12, 16, 18, 20, 23)

RADIATION PROTECTION PROGRAM

- I. Personnel Training
- II. Rules for safely handling a Sr-90 Eye Applicator
- III. Wipe Test
- IV. Waste Disposal

I. PERSONNEL TRAINING.

The Beta Eye Applicator can only be handled by the authorized user when treatments are performed or by the radiation physics consultant when leak testing procedures are being made. (Please see Item 8 for training and experience with radiation of the authorized user and the radiation physics consultant).

During treatments, paramedical personnel stay away from the source in such a manner that the total dose received by any one of those employees shall not exceed the maximum permissible dose for the general public.

II. RULES FOR SAFELY HANDLING A SR - 90 EYE APPLICATOR.

(Ref: Enclosure 2 - Information to be submitted when requesting possession and use of Sr-90 as Ophthalmic Applicator)

1. Wear your personnel dosimeter (s) if available, whenever you handle the Sr-90 Eye Applicator.
2. Remove the Sr-90 Eye Applicator from its secured storage location just before use. Do not leave it out any longer than necessary.
3. After removing the Applicator from its storage location,
 - a. Do not touch the treatment end of the applicator with your hands or other portion of your body.
 - b. Always hold the applicator by its handle.
 - c. Except during patient treatment, do not point the treatment end of the applicator toward another person, especially toward the eyes.
4. When the applicator is to be sterilized, place on a flat surface, use a cotton swab, sponge or gauze dampened with a sterilizing agent, then wipe the treatment end or the applicator across the swab, sponge or gauze. Do not sterilize by holding the swab or gauze in your hand.
5. During treatment, hold the patient's eye lids open with tape or other device, not with your fingers.
6. Immediately after treatment and/or resterilization, return the Sr-90 Eye Applicator to its storage container and to its secured location, i.e. keyed cabinet.

7. Do not remove any metal or plastic inserts from the manufacturer-supplied storage container. These items are generally a part of the container's shielding. Removal of these items can lead to excessive and unnecessary radiation exposures.
8. In event of apparent or probable damage to the source it shall immediately be placed into the storage container. The storage container shall be wrapped or placed into a plastic bag and secured. The cognizant radiation protection officer, regulatory agency, or the radiation physics consultant shall be contacted immediately for consultation and action.
9. In order to ensure that radiation exposures will be as low as reasonably achievable (ALARA), in the use and handling of the Sr-90 sealed source, the authorized user, Bernardo A. Puebla, M.D., enforces the following actions:
 - a. As soon as new staff members (e.g., physicians or other individuals who assist with patient treatments) report for duty and at least annually thereafter, it will be organized a refresher training in the rules for safe handling of the Sr-90 eye applicator and in the items specified in 10 CFR 19.12
 - b. At least once each year, both the authorized user and the radiation physics consultant will review the results of personnel monitoring if available, consider ways of reducing radiation exposures and implement needed changes in procedures, equipment, etc.

III. WIPE TESTS.

Perform routine wipe test at 6 - month intervals and maintain records. The source shall be withdrawn from service if leak test results indicate any increase in detectable activity from that of previous leak test. Removable contamination activity should be much less than 0.005 uCi.

Leak test shall be performed by persons specifically authorized by the Commission or an Agreement State to perform such services.

IV. WASTE DISPOSAL.

It is not foreseen any waste disposal in the proposed use and handling of the Sr-90 sealed source Eye Applicator. In the event of a serious damage to the applicator, the final disposal will be performed by the manufacturer, i.e. New England

Nuclear or any other licensee specifically approved to handle and/or dispose this source.