

Appendix

NOTICE OF VIOLATION

Appiewood Medical Center

License No. 24-24351-01

As a result of the inspection conducted on August 13, 1985, and in accordance with the General Policy and Procedures for NRC Enforcement Actions, (10 CFR Part 2, Appendix C), the following violations were identified:

1. License Condition No. 15 requires that licensed material be possessed and used in accordance with the statements, representations, and procedures contained in certain reference documents.

The referenced June 2, 1984 application states that TLD rings will be worn by individuals handling the Norland bone densitometer.

Contrary to the above, TLD rings were not worn by two individuals using the bone densitometer in 1984 and 1985.

This is a Severity Level IV violation (Supplement VI).

2. License Condition No. 15 requires that licensed material be possessed and used in accordance with the statements, representations, and procedures contained in certain referenced documents.

The referenced June 2, 1984 application states that survey instruments will be calibrated at least annually and will not be used beyond the calibration anniversary date.

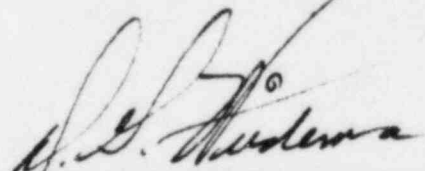
Contrary to this requirement, your Nuclear Associates survey instrument has not been calibrated at least since June 1984, and has been used subsequently (to date) for detection purposes.

This is a Severity Level IV violation (Supplement VI).

Pursuant to the provisions of 10 CFR 2.201, you are required to submit to this office within thirty days of the date of this Notice a written statement or explanation in reply, including for each item of noncompliance: (1) corrective action taken and the results achieved; (2) corrective action to be taken to avoid further noncompliance; and (3) the date when full compliance will be achieved. Consideration may be given to extending your response time for good cause shown.

SEP 16 1985

Dated \_\_\_\_\_

  
D. G. Wiedeman, Chief  
Nuclear Materials Safety  
Section 1

8509200012 850916  
REG3 LIC30  
24-24351-01 PDR